


LB116441

7470A

INSTRUMENT ID: CV2

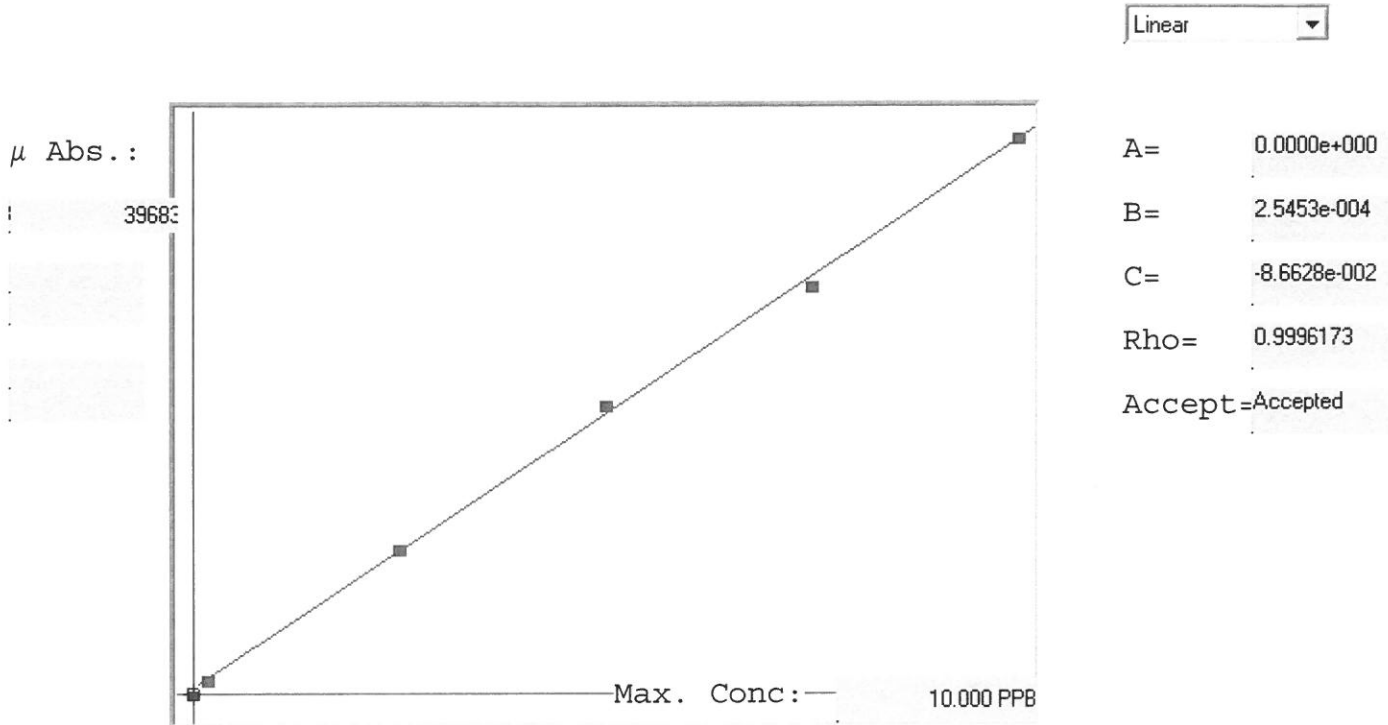

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	9/6/11
0.0	0.000	-0.067	-0.067	78	0.000	78					-9
0.2	0.200	0.183	-0.017	1060	0.0 %	1060					2
2.5	2.500	2.559	0.059	10396	0.0 %	10396					3
5.0	5.000	5.169	0.169	20650	0.0 %	20650					-2
7.5	7.500	7.341	-0.159	29181	0.0 %	29181					0
10.0	10.000	10.014	0.014	39683	0.0 %	39683					

LB116441 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 22 Sep 2021 14:08:23

Sample ID	Extended ID	μ Abs.	Conc.	Std. Conc	Method	Units	Date	Type	Type
0.0 - 1	50	78	-	0.0000	7470A	PPB	22 Sep 2021 14:11:33	S	Std
0.2 - 1	50.2	1060	-	0.2000	7470A	PPB	22 Sep 2021 14:13:50	S	Std
2.5 - 1	52.5	10396	-	2.5000	7470A	PPB	22 Sep 2021 14:16:07	S	Std
5.0 - 1	55	20650	-	5.0000	7470A	PPB	22 Sep 2021 14:18:24	S	Std
7.5 - 1	57.5	29181	-	7.5000	7470A	PPB	22 Sep 2021 14:20:41	S	Std
10.0 - 1	510	39683	-	10.0000	7470A	PPB	22 Sep 2021 14:25:28	S	Std
ICV05 - 1	ICV05	16503	4.1139	-	7470A	PPB	22 Sep 2021 14:28:35	U	SMPL
ICB05 - 1	ICB05	31	-0.0787	-	7470A	PPB	22 Sep 2021 14:30:50	U	SMPL
CCV95 - 1	CCV95	20779	5.2023	-	7470A	PPB	22 Sep 2021 14:33:04	U	SMPL
CCB95 - 1	CCB95	20	-0.0815	-	7470A	PPB	22 Sep 2021 14:35:20	U	SMPL
CRA - 1	CRA	1025	0.1743	-	7470A	PPB	22 Sep 2021 14:37:35	U	SMPL
HighStd - 1	HighStd	39290	9.9139	-	7470A	PPB	22 Sep 2021 14:44:20	U	SMPL
ChkStd - 1	ChkStd	26302	6.6080	-	7470A	PPB	22 Sep 2021 14:46:35	U	SMPL
PB139288BL - 1	PBW	-11	-0.0894	-	7470A	PPB	22 Sep 2021 14:48:51	U	SMPL
PB139288BS - 1	LCSW	17434	4.3509	-	7470A	PPB	22 Sep 2021 14:51:07	U	SMPL
M3835-07 - 1	SW-RR-02-(1.0)	-7	-0.0884	-	7470A	PPB	22 Sep 2021 14:53:23	U	SMPL
M3835-07DUP - 1	SW-RR-02-(1.0)DUP	34	-0.0780	-	7470A	PPB	22 Sep 2021 14:55:41	U	SMPL
M3835-07MS - 1	SW-RR-02-(1.0)MS	14959	3.7209	-	7470A	PPB	22 Sep 2021 14:57:58	U	SMPL
M3835-07MSD - 1	SW-RR-02-(1.0)MSD	14886	3.7023	-	7470A	PPB	22 Sep 2021 15:00:15	U	SMPL
M3835-08 - 1	SW-CB-03-(1.0)	463	0.0312	-	7470A	PPB	22 Sep 2021 15:02:31	U	SMPL
CCV96 - 1	CCV96	20211	5.0577	-	7470A	PPB	22 Sep 2021 15:04:46	U	SMPL
CCB96 - 1	CCB96	29	-0.0792	-	7470A	PPB	22 Sep 2021 15:07:01	U	SMPL
M3835-09 - 1	SW-CB-04-(1.0)	495	0.0394	-	7470A	PPB	22 Sep 2021 15:09:16	U	SMPL
M3835-10 - 1	SW-CB-02-(0.2)	271	-0.0177	-	7470A	PPB	22 Sep 2021 15:11:31	U	SMPL
M3835-11 - 1	SW-RR-01-(1.5)	95	-0.0624	-	7470A	PPB	22 Sep 2021 15:13:47	U	SMPL
M3871-04 - 1	FB02-BL	611	0.0689	-	7470A	PPB	22 Sep 2021 15:16:02	U	SMPL
M3835-07LX5 - 1		59	-0.0716	-	7470A	PPB	22 Sep 2021 15:18:18	U	SMPL
M3835-07A - 1		16374	4.0810	-	7470A	PPB	22 Sep 2021 15:20:34	U	SMPL
CCV97 - 1	CCV97	20528	5.1384	-	7470A	PPB	22 Sep 2021 15:22:51	U	SMPL
CCB97 - 1	CCB97	28	-0.0795	-	7470A	PPB	22 Sep 2021 15:25:07	U	SMPL