

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : pol

Instrument ID : Konelab

9/22/2021 14:07

Test: CNEPA-NEW

Sample Id	Result	Dil. 1 +	Response	Errors
ICV001 ICV001	94.169	0.0	0.112	
ICB001 ICB001	1.227	0.0	0.009	
CCV001 CCV001	240.922	0.0	0.275	
CCB001 CCB001	1.373	0.0	0.010	
P B139248BL PBS248	1.469	0.0	0.010	
M3756-01 MC0AA6	1.334	0.0	0.010	
M3756-02 MC0AA6D	1.352	0.0	0.010	
M3756-03 MC0AA6S	93.615	0.0	0.112	
M3756-04 MC0AH9	2.532	0.0	0.011	
M3756-05 MC0AJ3	1.458	0.0	0.010	
M3756-06 MC0AJ8	1.577	0.0	0.010	
M3756-07 MC0AL0	1.537	0.0	0.010	
M3756-08 MC0AL2	-0.182	0.0	0.008	
M3756-09 MC0AL3	0.284	0.0	0.008	
M3756-10 MC0AL5	0.320	0.0	0.008	
M3756-11 MC0AN6	0.166	0.0	0.008	
M3756-12 MC0AP0	-0.445	0.0	0.008	
M3756-13 MC0AP6	-0.382	0.0	0.008	
CCV002 CCV002	232.835	0.0	0.266	
CCB002 CCB002	1.738	0.0	0.010	
P B139264BL PBW264	1.554	0.0	0.010	
M3754-06 MC0AD3	1.137	0.0	0.009	
M3754-07 MC0AG0	-0.180	0.0	0.008	
M3754-08 MC0AG1	-0.505	0.0	0.007	
M3754-09 MC0AG6	-0.130	0.0	0.008	
M3754-10 MC0AF4	-0.404	0.0	0.008	
M3754-12 MC0AF7	-0.364	0.0	0.008	
M3754-13 MC0AF8	-0.407	0.0	0.008	
M3754-14 MC0AF9	-0.298	0.0	0.008	
M3754-15 MC0AF9D	-0.475	0.0	0.008	
M3754-16 MC0AF9S	96.618	0.0	0.115	
M3754-17 MC0AG2	0.021	0.0	0.008	
M3754-11 MC0AF6	2.692	0.0	0.011	
CCV003 CCV003	250.512	0.0	0.286	
CCB003 CCB003	1.702	0.0	0.010	

N	35
Mean	29.382
SD	71.0849
CV%	241.93

Aquakem v. 7.2AQ1

Results from time period:

Wed Sep 22 12:51:05 2021

Wed Sep 22 14:06:47 2021

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time
S0	A	CNEPA-NE\ P		1.3683	µg/l	9/22/2021 12:51:05
S5.0	A	CNEPA-NE\ P		4.3921	µg/l	9/22/2021 12:51:06
S10.0	A	CNEPA-NE\ P		9.7091	µg/l	9/22/2021 12:51:07
S100.0	A	CNEPA-NE\ P		99.2125	µg/l	9/22/2021 12:51:08
S250.0	A	CNEPA-NE\ P		250.2974	µg/l	9/22/2021 12:51:09
S500.0	A	CNEPA-NE\ P		500.0207	µg/l	9/22/2021 12:51:10
ICV001 ICV001	S	CNEPA-NE\ P		94.1689	µg/l	9/22/2021 13:29:26
ICB001 ICB001	S	CNEPA-NE\ P		1.2274	µg/l	9/22/2021 13:29:27
CCV001 CCV001	S	CNEPA-NE\ P		240.9221	µg/l	9/22/2021 13:29:29
CCB001 CCB001	S	CNEPA-NE\ P		1.373	µg/l	9/22/2021 13:29:32
PB139248BL PBS248	S	CNEPA-NE\ P		1.4686	µg/l	9/22/2021 13:29:34
M3756-01 MC0AA6	S	CNEPA-NE\ P		1.3336	µg/l	9/22/2021 13:29:35
M3756-02 MC0AA6D	S	CNEPA-NE\ P		1.3519	µg/l	9/22/2021 13:36:59
M3756-03 MC0AA6S	S	CNEPA-NE\ P		93.615	µg/l	9/22/2021 13:37:00
M3756-04 MC0AH9	S	CNEPA-NE\ P		2.5315	µg/l	9/22/2021 13:37:01
M3756-05 MC0AJ3	S	CNEPA-NE\ P		1.458	µg/l	9/22/2021 13:37:02
M3756-06 MC0AJ8	S	CNEPA-NE\ P		1.5767	µg/l	9/22/2021 13:37:03
M3756-07 MC0AL0	S	CNEPA-NE\ P		1.5368	µg/l	9/22/2021 13:37:04
M3756-08 MC0AL2	S	CNEPA-NE\ P		-0.1825	µg/l	9/22/2021 13:37:05
M3756-09 MC0AL3	S	CNEPA-NE\ P		0.2835	µg/l	9/22/2021 13:37:06
M3756-10 MC0AL5	S	CNEPA-NE\ P		0.3198	µg/l	9/22/2021 13:37:07
M3756-11 MC0AN6	S	CNEPA-NE\ P		0.1657	µg/l	9/22/2021 13:37:08
M3756-12 MC0AP0	S	CNEPA-NE\ P		-0.4446	µg/l	9/22/2021 13:37:09
M3756-13 MC0AP6	S	CNEPA-NE\ P		-0.3818	µg/l	9/22/2021 13:44:32
CCV002 CCV002	S	CNEPA-NE\ P		232.8353	µg/l	9/22/2021 13:44:33
CCB002 CCB002	S	CNEPA-NE\ P		1.7383	µg/l	9/22/2021 13:44:34
PB139264BL PBW264	S	CNEPA-NE\ P		1.5541	µg/l	9/22/2021 13:44:35
M3754-06 MC0AD3	S	CNEPA-NE\ P		1.1366	µg/l	9/22/2021 13:44:36
M3754-07 MC0AG0	S	CNEPA-NE\ P		-0.1798	µg/l	9/22/2021 13:44:37
M3754-08 MC0AG1	S	CNEPA-NE\ P		-0.5053	µg/l	9/22/2021 13:44:38
M3754-09 MC0AG6	S	CNEPA-NE\ P		-0.1297	µg/l	9/22/2021 13:44:39
M3754-10 MC0AF4	S	CNEPA-NE\ P		-0.404	µg/l	9/22/2021 13:44:40
M3754-12 MC0AF7	S	CNEPA-NE\ P		-0.3643	µg/l	9/22/2021 13:44:42
M3754-13 MC0AF8	S	CNEPA-NE\ P		-0.4073	µg/l	9/22/2021 13:50:15
M3754-14 MC0AF9	S	CNEPA-NE\ P		-0.2977	µg/l	9/22/2021 13:50:16
M3754-15 MC0AF9D	S	CNEPA-NE\ P		-0.4755	µg/l	9/22/2021 13:50:17
M3754-16 MC0AF9S	S	CNEPA-NE\ P		96.6184	µg/l	9/22/2021 13:50:18
M3754-17 MC0AG2	S	CNEPA-NE\ P		0.021	µg/l	9/22/2021 13:50:19
M3754-11 MC0AF6	S	CNEPA-NE\ P		2.692	µg/l	9/22/2021 14:06:43
CCV003 CCV003	S	CNEPA-NE\ P		250.5123	µg/l	9/22/2021 14:06:44
CCB003 CCB003	S	CNEPA-NE\ P		1.7023	µg/l	9/22/2021 14:06:47

CHEMTECH CONSULTING GROUP INC

284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : AB

Instrument ID : Konelab

9/22/2021 12:51

Test CNEPA-NEW

Accepted

9/22/2021 12:51

Factor slope

902 0.001109

AB

Bias y-intercept


0.008

9/22/21

Coeff. of det.

0.999985

Errors

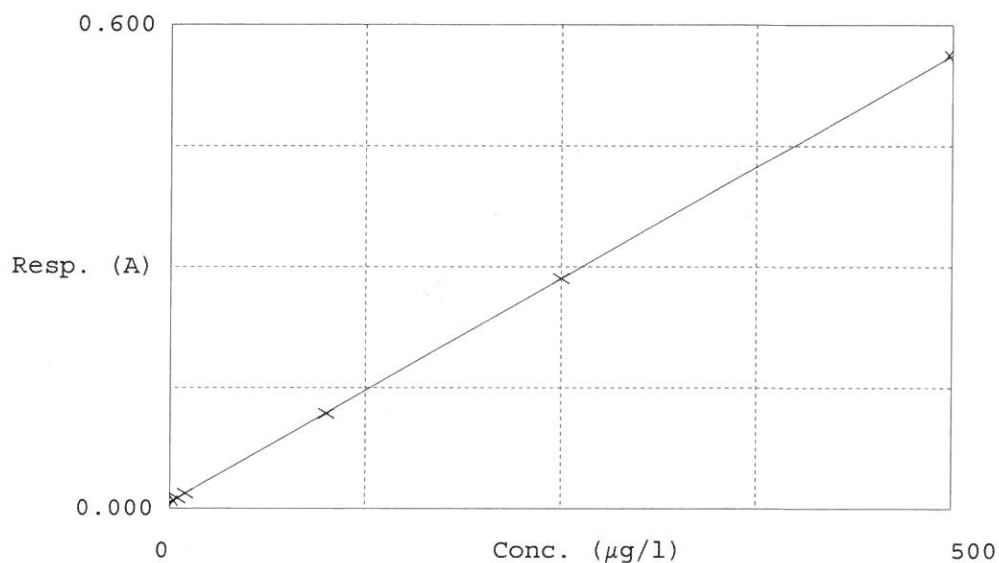

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN 50.0	0.010	1.3683	0.0000	
2	5.0PPBCN 5.0	0.013	4.3921	5.0000	
3	10PPBCN 10.0	0.019	9.7091	10.0000	
4	100PPBCN 100.0	0.118	99.2125	100.0000	
5	250PPBCN 250.0	0.286	250.2974	250.0000	
6	500PPBCN 500.0	0.562	500.0207	500.0000	

Rel

Errors

$\bar{12.2}$
 $\bar{2.9}$
 $\bar{0.8}$
 $\bar{0.1}$
 $\bar{0.0}$

AB

9/22/21