


LB116473

7470A

INSTRUMENT ID: CV1

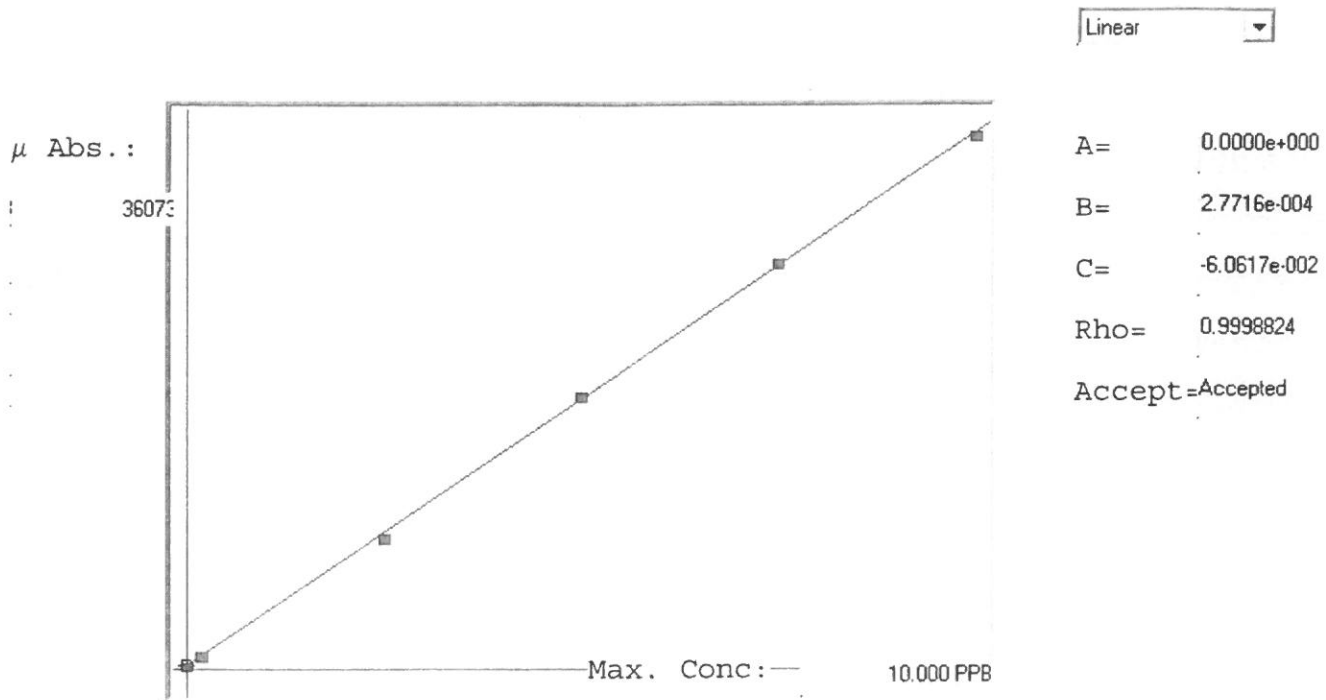

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	0.017	0.017	279	0.000	279					-
0.2	0.200	0.196	-0.004	925	0.0 %	925					-2
2.5	2.500	2.420	-0.080	8949	0.0 %	8949					-3
5.0	5.000	5.068	0.068	18504	0.0 %	18504					1
7.5	7.500	7.563	0.063	27505	0.0 %	27505					1
10.0	10.000	9.937	-0.063	36073	0.0 %	36073					-1

LB116473 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 23 Sep 2021 13:38:34

Sample ID	Extended ID	μ Abs	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	279	-	0.0000	7470A	PPB	23 Sep 2021 13:40:14	S	Std
0.2 - 1	50.2	925	-	0.2000	7470A	PPB	23 Sep 2021 13:42:31	S	Std
2.5 - 1	52.5	8949	-	2.5000	7470A	PPB	23 Sep 2021 13:44:48	S	Std
5.0 - 1	55	18504	-	5.0000	7470A	PPB	23 Sep 2021 13:47:05	S	Std
7.5 - 1	57.5	27505	-	7.5000	7470A	PPB	23 Sep 2021 13:49:22	S	Std
10.0 - 1	51.5	36073	-	10.0000	7470A	PPB	23 Sep 2021 13:54:20	S	Std
ICV09 - 1	ICV09	14026	3.8268	-	7470A	PPB	23 Sep 2021 13:57:00	U	SMPL
ICB09 - 1	ICB09	178	-0.0113	-	7470A	PPB	23 Sep 2021 14:01:55	U	SMPL
CCV07 - 1	CCV07	18953	5.1924	-	7470A	PPB	23 Sep 2021 14:04:09	U	SMPL
CCB07 - 1	CCB07	148	-0.0196	-	7470A	PPB	23 Sep 2021 14:06:24	U	SMPL
CRA - 1	CRA	838	0.1716	-	7470A	PPB	23 Sep 2021 14:08:40	U	SMPL
HighStd - 1	HighStd	35859	9.8780	-	7470A	PPB	23 Sep 2021 14:10:55	U	SMPL
ChkStd - 1	ChkStd	26015	7.1497	-	7470A	PPB	23 Sep 2021 14:13:10	U	SMPL
PB139314BL - 1	PBW	336	0.0325	-	7470A	PPB	23 Sep 2021 14:18:06	U	SMPL
PB139314BS - 1	LCSW	14532	3.9670	-	7470A	PPB	23 Sep 2021 14:20:21	U	SMPL
M3832-02 - 1	TP-B	23	-0.0542	-	7470A	PPB	23 Sep 2021 14:22:37	U	SMPL
M3860-03 - 1	PT-SOIL	178	-0.0113	-	7470A	PPB	23 Sep 2021 14:24:55	U	SMPL
M3870-02 - 1	TP-C	238	0.0053	-	7470A	PPB	23 Sep 2021 14:27:12	U	SMPL
M3872-02 - 1	SP-LPA-01	852	0.1755	-	7470A	PPB	23 Sep 2021 14:29:29	U	SMPL
M3872-02DUP - 1	SP-LPA-01DUP	803	0.1619	-	7470A	PPB	23 Sep 2021 14:31:45	U	SMPL
CCV08 - 1	CCV08	18609	5.0970	-	7470A	PPB	23 Sep 2021 14:34:00	U	SMPL
CCB08 - 1	CCB08	90	-0.0357	-	7470A	PPB	23 Sep 2021 14:36:16	U	SMPL
M3872-02MS - 1	SP-LPA-01MS	15658	4.2791	-	7470A	PPB	23 Sep 2021 14:38:32	U	SMPL
M3872-02MSD - 1	SP-LPA-01MSD	15721	4.2966	-	7470A	PPB	23 Sep 2021 14:40:47	U	SMPL
PB139315BL - 1	PBW	152	-0.0185	-	7470A	PPB	23 Sep 2021 14:43:03	U	SMPL
PB139315BS - 1	LCSW	14410	3.9332	-	7470A	PPB	23 Sep 2021 14:45:19	U	SMPL
M3875-15 - 1	20882	1673	0.4031	-	7470A	PPB	23 Sep 2021 14:52:24	U	SMPL
M3875-15DUP - 1	20882DUP	1514	0.3590	-	7470A	PPB	23 Sep 2021 14:54:40	U	SMPL
M3875-15MS - 1	20882MS	15056	4.1123	-	7470A	PPB	23 Sep 2021 14:56:56	U	SMPL
M3875-15MSD - 1	20882MSD	14528	3.9659	-	7470A	PPB	23 Sep 2021 14:59:13	U	SMPL
CCV09 - 1	CCV09	19181	5.2556	-	7470A	PPB	23 Sep 2021 15:01:29	U	SMPL
CCB09 - 1	CCB09	189	-0.0082	-	7470A	PPB	23 Sep 2021 15:03:45	U	SMPL
RB139314TB - 1	PB139278TB	252	0.0092	-	7470A	PPB	23 Sep 2021 15:06:00	U	SMPL
M3872-02LX5 - 1		91	-0.0354	-	7470A	PPB	23 Sep 2021 15:08:16	U	SMPL
M3872-02A - 1		15115	4.1286	-	7470A	PPB	23 Sep 2021 15:10:31	U	SMPL
M3875-15LX5 - 1		340	0.0336	-	7470A	PPB	23 Sep 2021 15:12:47	U	SMPL
M3875-15A - 1		15844	4.3307	-	7470A	PPB	23 Sep 2021 15:15:02	U	SMPL
CCV10 - 1	CCV10	19499	5.3437	-	7470A	PPB	23 Sep 2021 15:17:18	U	SMPL
CCB10 - 1	CCB10	251	0.0089	-	7470A	PPB	23 Sep 2021 15:19:33	U	SMPL