


LB116488

7470A

INSTRUMENT ID: CV1

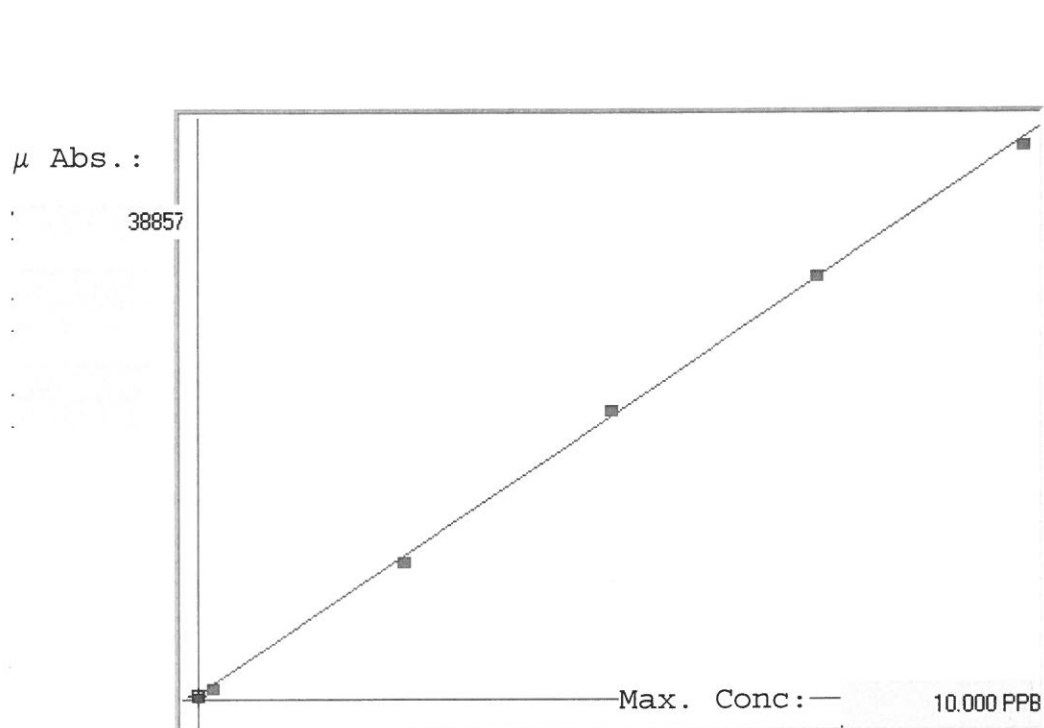

Linear

A= 0.0000e+000

B= 2.5647e-004

C= -7.1818e-002

Rho= 0.9997457

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	-0.002	-0.002	272	0.000	272					-19
0.2	0.200	0.163	-0.037	916	0.0 %	916					-3
2.5	2.500	2.439	-0.061	9789	0.0 %	9789					3
5.0	5.000	5.147	0.147	20348	0.0 %	20348					1
7.5	7.500	7.560	0.060	29757	0.0 %	29757					-1
10.0	10.000	9.894	-0.106	38857	0.0 %	38857					

LB116488 INSTRUMENT ID : CV1

Method: 7470A		Operator: Admin		Date of Analysis: 23 Sep 2021 18:16:14					
Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	272	-	0.0007	7470A	PPB	23 Sep 2021	18:23:20	S Std
0.2 - 1	50.2	916	-	0.2000	7470A	PPB	23 Sep 2021	18:25:37	S Std
2.5 - 1	52.5	9789	-	2.5000	7470A	PPB	23 Sep 2021	18:27:54	S Std
5.0 - 1	55	20348	-	5.0000	7470A	PPB	23 Sep 2021	18:30:11	S Std
7.5 - 1	57.5	29757	-	7.5000	7470A	PPB	23 Sep 2021	18:32:28	S Std
10.0 - 1	510	38857	-	10.0000	7470A	PPB	23 Sep 2021	18:34:43	S Std
ICV11 - 1	ICV11	15791	3.9780	-	7470A	PPB	23 Sep 2021	18:37:31	U SMPL
ICB11 - 1	ICB11	87	-0.0495	-	7470A	PPB	23 Sep 2021	18:39:45	U SMPL
CCV14 - 1	CCV14	20298	5.1339	-	7470A	PPB	23 Sep 2021	18:42:00	U SMPL
CCB14 - 1	CCB14	204	-0.0195	-	7470A	PPB	23 Sep 2021	18:46:49	U SMPL
CRA - 1	CRA	1000	0.1846	-	7470A	PPB	23 Sep 2021	18:51:33	U SMPL
HighStd - 1	HighStd	38047	9.6859	-	7470A	PPB	23 Sep 2021	18:53:48	U SMPL
ChkStd - 1	ChkStd	26327	6.6801	-	7470A	PPB	23 Sep 2021	18:56:03	U SMPL
PB139332BL - 1	PBW	137	-0.0367	-	7470A	PPB	23 Sep 2021	19:01:39	U SMPL
PB139332BS - 1	LCSW	14564	3.6633	-	7470A	PPB	23 Sep 2021	19:03:55	U SMPL
M3752-01 - 1	FB-1P	3395	0.7989	-	7470A	PPB	23 Sep 2021	19:06:11	U SMPL
M3911-01 - 1	SW-RR-02-(1.0)	39	-0.0618	-	7470A	PPB	23 Sep 2021	19:08:28	U SMPL
M3911-02 - 1	SW-RR-01-(2.0)	187	-0.0239	-	7470A	PPB	23 Sep 2021	19:10:45	U SMPL
M3911-03 - 1	SW-RR-03-(SA)	130	-0.0385	-	7470A	PPB	23 Sep 2021	19:13:02	U SMPL
M3911-04 - 1	SW-CB-02-(0.2)	108	-0.0441	-	7470A	PPB	23 Sep 2021	19:15:18	U SMPL
CCV15 - 1	CCV15	19208	4.8544	-	7470A	PPB	23 Sep 2021	19:17:34	U SMPL
CCB15 - 1	CCB15	96	-0.0472	-	7470A	PPB	23 Sep 2021	19:19:49	U SMPL
M3911-05 - 1	SW-CB-04-(0.5)	1298	0.2611	-	7470A	PPB	23 Sep 2021	19:22:04	U SMPL
M3911-05DUP - 1	SW-CB-04-(0.5)DUP	1224	0.2421	-	7470A	PPB	23 Sep 2021	19:24:19	U SMPL
M3911-06 - 1	M3911-05MS	15113	3.8041	-	7470A	PPB	23 Sep 2021	19:26:35	U SMPL
M3911-07 - 1	M3911-05MSD	14914	3.7531	-	7470A	PPB	23 Sep 2021	19:28:50	U SMPL
M3911-16 - 1	P287-DITCH	109	-0.0439	-	7470A	PPB	23 Sep 2021	19:31:06	U SMPL
M3914-05 - 1	LV-TOTES	122	-0.0405	-	7470A	PPB	23 Sep 2021	19:33:23	U SMPL
M3911-05LX5 - 1		420	0.0359	-	7470A	PPB	23 Sep 2021	19:35:40	U SMPL
M3911-05A - 1		16059	4.0468	-	7470A	PPB	23 Sep 2021	19:37:56	U SMPL
CCV16 - 1	CCV16	20095	5.0819	-	7470A	PPB	23 Sep 2021	19:40:14	U SMPL
CCB16 - 1	CCB16	70	-0.0539	-	7470A	PPB	23 Sep 2021	19:42:29	U SMPL