

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : ml Instrument ID : Konelab

9/24/2021 9:52

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	96.363	0.0	0.084	
ICB1	-0.379	0.0	0.001	
CCV1	246.017	0.0	0.212	
CCB1	-0.342	0.0	0.001	
PB139325BL	-0.539	0.0	0.001	
PB139325BS	95.881	0.0	0.083	
LOWPB139325	9.534	0.0	0.009	
HIGHPB139325	481.699	0.0	0.415	
M3870-01	0.571	0.0	0.002	
M3870-01DUP	0.288	0.0	0.001	
M3870-01MS	30.983	0.0	0.028	
M3870-01MSD	31.401	0.0	0.028	
M3872-01	23.235	0.0	0.021	
CCV2	248.416	0.0	0.214	
CCB2	0.991	0.0	0.002	

N	15
Mean	84.275
SD	138.5624
CV%	164.42

- 757 (90-110)
- 767
ml
9/24/21

Aquakem v. 7.2AQ1

Results from time period:

Fri Sep 24 09:05:35 2021

Fri Sep 24 10:05:48 2021

Sample Id	Sam/Ctr/c	Test short	Test type	Result	Result unit	Result date and time	Stat
0.0PPBCN	A	Total CN	P	-0.1708	µg/l	9/24/2021 9:05:35	
5.0PPBCN	A	Total CN	P	4.7336	µg/l	9/24/2021 9:05:36	
10PPBCN	A	Total CN	P	9.0307	µg/l	9/24/2021 9:05:37	
50PPBCN	A	Total CN	P	48.6216	µg/l	9/24/2021 9:05:38	
100PPBCN	A	Total CN	P	100.7514	µg/l	9/24/2021 9:05:39	
250PPBCN	A	Total CN	P	254.0479	µg/l	9/24/2021 9:05:40	
500PPBCN	A	Total CN	P	497.9856	µg/l	9/24/2021 9:05:41	
ICV1	S	Total CN	P	96.3628	µg/l	9/24/2021 9:43:14	
ICB1	S	Total CN	P	-0.379	µg/l	9/24/2021 9:43:16	
CCV1	S	Total CN	P	246.0172	µg/l	9/24/2021 9:43:18	
CCB1	S	Total CN	P	-0.3422	µg/l	9/24/2021 9:43:19	
PB139325BL	S	Total CN	P	-0.5388	µg/l	9/24/2021 9:43:22	
PB139325BS	S	Total CN	P	95.8811	µg/l	9/24/2021 9:43:23	
LOWPB139325	S	Total CN	P	9.5341	µg/l	9/24/2021 9:50:45	
HIGHPB139325	S	Total CN	P	481.6989	µg/l	9/24/2021 9:50:46	
M3870-01	S	Total CN	P	0.5709	µg/l	9/24/2021 9:50:47	
M3870-01DUP	S	Total CN	P	0.2884	µg/l	9/24/2021 9:50:48	
M3870-01MS	S	Total CN	P	30.9825	µg/l	9/24/2021 9:50:51	
M3870-01MSD	S	Total CN	P	31.4006	µg/l	9/24/2021 9:50:52	
M3872-01	S	Total CN	P	23.2351	µg/l	9/24/2021 9:50:53	
CCV2	S	Total CN	P	248.4162	µg/l	9/24/2021 9:50:54	
CCB2	S	Total CN	P	0.9909	µg/l	9/24/2021 9:50:55	

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : AL

Instrument ID : Konelab

9/24/2021 9:07


Test Total CN

Accepted 9/24/2021 9:07

Factor 1165
Bias 0.001

Coeff. of det. 0.999883

Errors

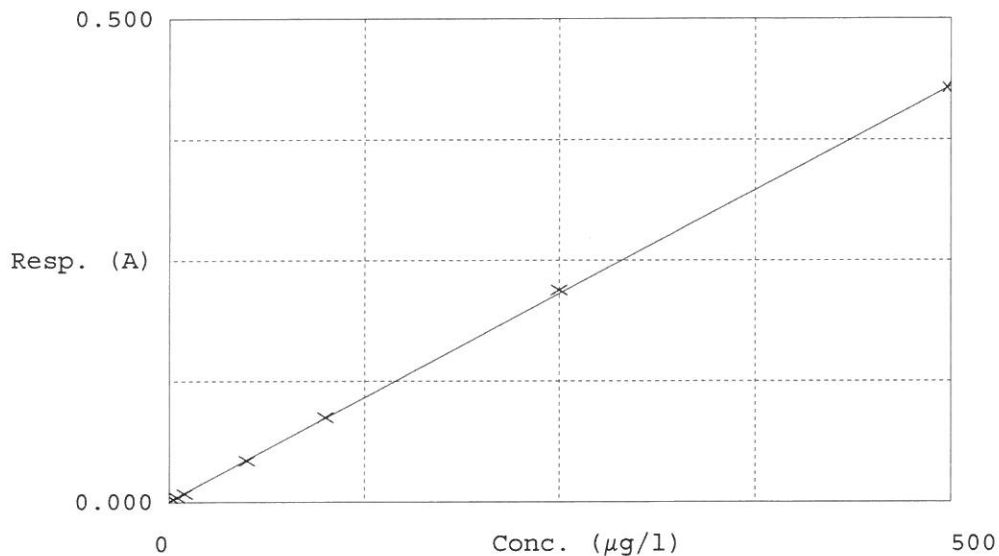

	Calibrator	Response	Calc. con.	Conc.	Rel. Errors
1	0.0PPBCN	0.001	-0.1708	0.0000	0
2	5.0PPBCN	0.005	4.7336	5.0000	-5.3
3	10PPBCN	0.009	9.0307	10.0000	-9.7
4	50PPBCN	0.043	48.6216	50.0000	-2.8
5	100PPBCN	0.088	100.7514	100.0000	0.8
6	250PPBCN	0.219	254.0479	250.0000	1.6
7	500PPBCN	0.428	497.9856	500.0000	-0.4

AT
9/24/21