


LB116529

7471B

INSTRUMENT ID: CV1

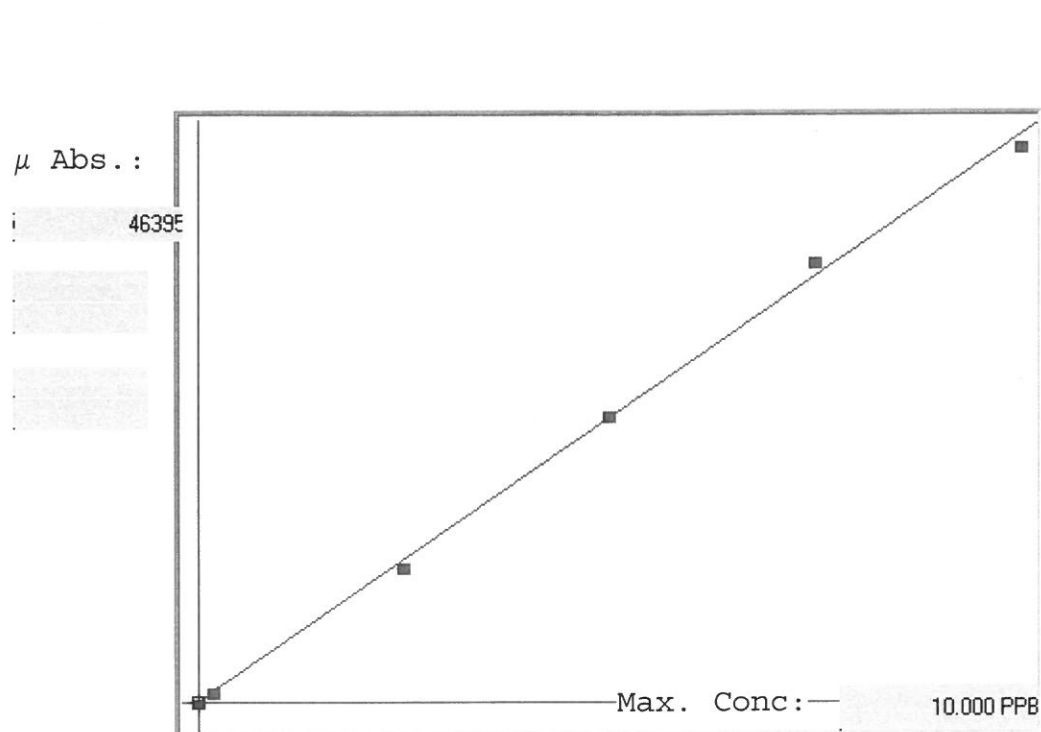

Linear

A= 0.0000e+000

B= 2.1102e-004

C= -7.4685e-003

Rho= 0.9991255

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%))
0.0	0.000	0.021	0.021	133	0.000	133					-
0.2	0.200	0.191	-0.009	942	0.0 %	942					-5
2.5	2.500	2.372	-0.128	11274	0.0 %	11274					-5
5.0	5.000	5.060	0.060	24016	0.0 %	24016					1
7.5	7.500	7.774	0.274	36875	0.0 %	36875					4
10.0	10.000	9.783	-0.217	46395	0.0 %	46395					-2

LB116529 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 27 Sep 2021 13:37:17

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	133	-	0.00007471B	PPB		27 Sep 2021 13:38:12	S	Std
0.2 - 1	50.2	942	-	0.20007471B	PPB		27 Sep 2021 13:40:30	S	Std
2.5 - 1	52.5	11274	-	2.50007471B	PPB		27 Sep 2021 13:42:47	S	Std
5.0 - 1	55	24016	-	5.00007471B	PPB		27 Sep 2021 13:45:04	S	Std
7.5 - 1	57.5	36875	-	7.50007471B	PPB		27 Sep 2021 13:47:20	S	Std
10.0 - 1	59	46395	-	10.00007471B	PPB		27 Sep 2021 13:54:53	S	Std
ICV13 - 1	ICV13	18119	3.8159	-7471B	PPB		27 Sep 2021 14:02:43	U	SMPL
ICB13 - 1	ICB13	58	0.0048	-7471B	PPB		27 Sep 2021 14:04:58	U	SMPL
CCV20 - 1	CCV20	24142	5.0869	-7471B	PPB		27 Sep 2021 14:07:14	U	SMPL
CCB20 - 1	CCB20	-2	-0.0079	-7471B	PPB		27 Sep 2021 14:09:29	U	SMPL
CRA - 1	CRA	922	0.1871	-7471B	PPB		27 Sep 2021 14:11:45	U	SMPL
HighStd - 1	HighStd	47073	9.9257	-7471B	PPB		27 Sep 2021 14:14:01	U	SMPL
ChkStd - 1	ChkStd	34295	7.2293	-7471B	PPB		27 Sep 2021 14:16:16	U	SMPL
PB139413BL - 1	PBS	-136	-0.0362	-7471B	PPB		27 Sep 2021 14:18:33	U	SMPL
PB139413BS - 1	LCSS	17817	3.7522	-7471B	PPB		27 Sep 2021 14:23:33	U	SMPL
M3906-01 - 1	BS-DRUM-COMP	1556	0.3209	-7471B	PPB		27 Sep 2021 14:25:49	U	SMPL
M3907-01 - 1	RT-3032	3873	0.8098	-7471B	PPB		27 Sep 2021 14:28:06	U	SMPL
M3907-03 - 1	RO-206	2671	0.5562	-7471B	PPB		27 Sep 2021 14:30:23	U	SMPL
M3913-01 - 1	TR-05-092321	3097	0.6460	-7471B	PPB		27 Sep 2021 14:32:39	U	SMPL
M3914-01 - 1	LV-DRUM-SOIL	728	0.1462	-7471B	PPB		27 Sep 2021 14:34:55	U	SMPL
CCV21 - 1	CCV21	24093	5.0765	-7471B	PPB		27 Sep 2021 14:37:10	U	SMPL
CCB21 - 1	CCB21	-11	-0.0098	-7471B	PPB		27 Sep 2021 14:39:26	U	SMPL
M3916-01 - 1	CONC-1	1886	0.3905	-7471B	PPB		27 Sep 2021 14:41:41	U	SMPL
M3916-04 - 1	CONC-2	393	0.0755	-7471B	PPB		27 Sep 2021 14:43:56	U	SMPL
M3916-07 - 1	CONC-3	406	0.0782	-7471B	PPB		27 Sep 2021 14:46:12	U	SMPL
M3916-10 - 1	CONC-4	473	0.0923	-7471B	PPB		27 Sep 2021 14:48:28	U	SMPL
M3916-13 - 1	BRICK-1	322	0.0605	-7471B	PPB		27 Sep 2021 14:50:44	U	SMPL
M3917-01 - 1	TP-3	10105	2.1248	-7471B	PPB		27 Sep 2021 14:53:00	U	SMPL
M3917-04 - 1	TP-6	6442	1.3519	-7471B	PPB		27 Sep 2021 14:55:17	U	SMPL
M3917-07 - 1	TP-10	11169	2.3494	-7471B	PPB		27 Sep 2021 14:57:34	U	SMPL
M3917-10 - 1	TP-9	10199	2.1447	-7471B	PPB		27 Sep 2021 14:59:51	U	SMPL
M3917-13 - 1	TP-8	3749	0.7836	-7471B	PPB		27 Sep 2021 15:02:06	U	SMPL
CCV22 - 1	CCV22	24673	5.1989	-7471B	PPB		27 Sep 2021 15:04:22	U	SMPL
CCB22 - 1	CCB22	-31	-0.0140	-7471B	PPB		27 Sep 2021 15:06:37	U	SMPL
M3917-16 - 1	TP-4	11467	2.4122	-7471B	PPB		27 Sep 2021 15:08:53	U	SMPL
M3917-19 - 1	TP-1	6860	1.4401	-7471B	PPB		27 Sep 2021 15:11:08	U	SMPL
M3921-01 - 1	SPOILS-REPORT-1	765	0.1540	-7471B	PPB		27 Sep 2021 15:13:24	U	SMPL
M3921-01DUP - 1	SPOILS-REPORT-1DUP	868	0.1757	-7471B	PPB		27 Sep 2021 15:15:40	U	SMPL
M3921-01MS - 1	SPOILS-REPORT-1MS	20680	4.3563	-7471B	PPB		27 Sep 2021 15:17:55	U	SMPL
M3921-01MSD - 1	SPOILS-REPORT-1MSD	20915	4.4059	-7471B	PPB		27 Sep 2021 15:20:11	U	SMPL
PB139414BL - 1	PBS	264	0.0482	-7471B	PPB		27 Sep 2021 15:22:28	U	SMPL
PB139414BS - 1	LCSS	19052	4.0128	-7471B	PPB		27 Sep 2021 15:24:45	U	SMPL
M3927-13 - 1	WOOSPK-BACKFILL-01	635	0.1265	-7471B	PPB		27 Sep 2021 15:27:01	U	SMPL
M3927-15 - 1	WOOSPK-BACKFILL-02	349	0.0662	-7471B	PPB		27 Sep 2021 15:29:17	U	SMPL
CCV23 - 1	CCV23	24524	5.1675	-7471B	PPB		27 Sep 2021 15:34:36	U	SMPL
CCB23 - 1	CCB23	-32	-0.0142	-7471B	PPB		27 Sep 2021 15:36:52	U	SMPL
M3939-02 - 1	TS-1	2413	0.5017	-7471B	PPB		27 Sep 2021 15:39:08	U	SMPL
M3939-02DUP - 1	TS-1DUP	2213	0.4595	-7471B	PPB		27 Sep 2021 15:41:23	U	SMPL
M3939-02MS - 1	TS-1MS	22952	4.8358	-7471B	PPB		27 Sep 2021 15:43:39	U	SMPL
M3939-02MSD - 1	TS-1MSD	24219	5.1031	-7471B	PPB		27 Sep 2021 15:45:54	U	SMPL
M3927-17 - 1	WOOSPK-BACKFILL-03	332	0.0626	-7471B	PPB		27 Sep 2021 15:48:10	U	SMPL
M3927-19 - 1	WOOSPK-BACKFILL-04	334	0.0630	-7471B	PPB		27 Sep 2021 15:50:27	U	SMPL
M3927-21 - 1	WOOSPK-BACKFILL-05	243	0.0438	-7471B	PPB		27 Sep 2021 15:52:43	U	SMPL
M3927-23 - 1	WOOSPK-BACKFILL-06	724	0.1453	-7471B	PPB		27 Sep 2021 15:55:00	U	SMPL
M3934-01 - 1	TP-5	3444	0.7193	-7471B	PPB		27 Sep 2021 15:57:17	U	SMPL
M3934-04 - 1	TP-7	7440	1.5625	-7471B	PPB		27 Sep 2021 15:59:32	U	SMPL
CCV24 - 1	CCV24	23793	5.0132	-7471B	PPB		27 Sep 2021 16:01:48	U	SMPL
CCB24 - 1	CCB24	-22	-0.0121	-7471B	PPB		27 Sep 2021 16:04:03	U	SMPL
M3934-07 - 1	TP-2	7117	1.4943	-7471B	PPB		27 Sep 2021 16:06:19	U	SMPL
M3935-01 - 1	TP-2	5232	1.0966	-7471B	PPB		27 Sep 2021 16:08:35	U	SMPL
M3935-04 - 1	TP-1-S	3113	0.6494	-7471B	PPB		27 Sep 2021 16:10:50	U	SMPL
M3941-01 - 1	124019	4595	0.9621	-7471B	PPB		27 Sep 2021 16:13:06	U	SMPL
M3941-03 - 1	124042	5056	1.0594	-7471B	PPB		27 Sep 2021 16:15:21	U	SMPL
M3943-01 - 1	WC-DB-1	8249	1.7332	-7471B	PPB		27 Sep 2021 16:17:38	U	SMPL
M3943-04 - 1	WC-TV-1	343492	72.4746	-7471B	PPB		27 Sep 2021 16:19:54	U	SMPL
M3944-01 - 1	BOILER-PIT-3-5	54425	11.4770	-7471B	PPB		27 Sep 2021 16:22:11	U	SMPL
M3946-01 - 1	PL-05-092421	1534	0.3162	-7471B	PPB		27 Sep 2021 16:24:31	U	SMPL
M3947-01 - 1	CL-02-092421	1003	0.2042	-7471B	PPB		27 Sep 2021 16:26:48	U	SMPL
CCV25 - 1	CCV25	23140	4.8754	-7471B	PPB		27 Sep 2021 16:29:04	U	SMPL
CCB25 - 1	CCB25	-13	-0.0102	-7471B	PPB		27 Sep 2021 16:31:20	U	SMPL
M3950-01 - 1	HD-02-092421	2150	0.4462	-7471B	PPB		27 Sep 2021 16:33:36	U	SMPL
M3921-01LX5 - 1		111	0.0160	-7471B	PPB		27 Sep 2021 16:35:53	U	SMPL
M3921-01A - 1		20987	4.4211	-7471B	PPB		27 Sep 2021 16:38:08	U	SMPL
M3939-02LX5 - 1		370	0.0706	-7471B	PPB		27 Sep 2021 16:40:24	U	SMPL
M3939-02A - 1		23407	4.9318	-7471B	PPB		27 Sep 2021 16:42:40	U	SMPL
M3943-04DLX10 - 1		40457	8.5296	-7471B	PPB		27 Sep 2021 16:44:56	U	SMPL
M3944-01DLX2 - 1		27520	5.7997	-7471B	PPB		27 Sep 2021 16:47:12	U	SMPL
CCV26 - 1	CCV26	24404	5.1421	-7471B	PPB		27 Sep 2021 16:52:03	U	SMPL
CCB26 - 1	CCB26	-24	-0.0125	-7471B	PPB		27 Sep 2021 16:54:20	U	SMPL