

LB 116567

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC

284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : AB Instrument ID : Konelab

9/29/2021 11:38

Test: ~~Total~~ CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	96.665	0.0	0.084	
ICB1	0.571	0.0	0.001	
CCV1	245.000	0.0	0.213	
CCB1	0.554	0.0	0.001	
PB139461BL	0.374	0.0	0.001	
M3951-02	0.443	0.0	0.001	
M3951-02DUP	0.652	0.0	0.001	
M3971-02	0.505	0.0	0.001	
M3971-08	0.529	0.0	0.001	
M3971-11	0.523	0.0	0.001	
M3971-05	0.420	0.0	0.001	
CCV2	259.872	0.0	0.226	
CCB2	0.630	0.0	0.001	

N	13
Mean	46.672
SD	95.1260
CV%	203.82

Aquakem v. 7.2AQ1

Results from time period:

Wed Sep 29 11:16:40 2021

Wed Sep 29 11:35:14 2021

Sample Id	Sam/Ctr/c	Test short name	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Reactive CN	P	-0.4668	µg/l	9/29/2021 8:42:18	
5.OPPBCN	A	Reactive CN	P	4.6781	µg/l	9/29/2021 8:42:19	
10PPBCN	A	Reactive CN	P	9.9793	µg/l	9/29/2021 8:42:20	
50PPBCN	A	Reactive CN	P	48.9331	µg/l	9/29/2021 8:42:21	
100PPBCN	A	Reactive CN	P	100.6416	µg/l	9/29/2021 8:42:22	
250PPBCN	A	Reactive CN	P	252.5052	µg/l	9/29/2021 8:42:23	
500PPBCN	A	Reactive CN	P	498.7294	µg/l	9/29/2021 8:42:24	
ICV1	S	Reactive CN	P	96.6655	µg/l	9/29/2021 11:16:40	
ICB1	S	Reactive CN	P	0.571	µg/l	9/29/2021 11:16:41	
CCV1	S	Reactive CN	P	244.9997	µg/l	9/29/2021 11:16:42	
CCB1	S	Reactive CN	P	0.5543	µg/l	9/29/2021 11:16:43	
PB139461BL	S	Reactive CN	P	0.3739	µg/l	9/29/2021 11:16:44	
M3951-02	S	Reactive CN	P	0.4429	µg/l	9/29/2021 11:16:45	
M3951-02DUP	S	Reactive CN	P	0.6518	µg/l	9/29/2021 11:16:46	
M3971-02	S	Reactive CN	P	0.5051	µg/l	9/29/2021 11:16:47	
M3971-08	S	Reactive CN	P	0.5288	µg/l	9/29/2021 11:16:49	
M3971-11	S	Reactive CN	P	0.5226	µg/l	9/29/2021 11:16:50	
M3971-05	S	Reactive CN	P	0.4202	µg/l	9/29/2021 11:32:39	
CCV2	S	Reactive CN	P	259.8718	µg/l	9/29/2021 11:35:13	
CCB2	S	Reactive CN	P	0.6298	µg/l	9/29/2021 11:35:14	

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : AS

Instrument ID : Konelab

9/29/2021 8:42


Test Total CN

Accepted 9/29/2021 8:42

Factor 1154
Bias 0

Coeff. of det. 0.999952

Errors

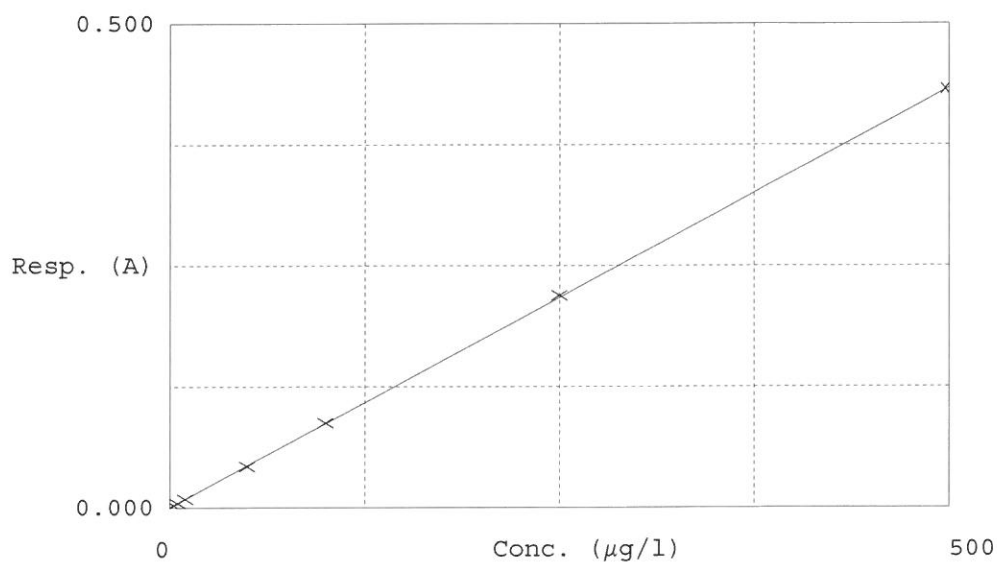

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.000	-0.4668	0.0000	-0.4
2	5.0PPBCN	0.005	4.6781	5.0000	-0.2
3	10PPBCN	0.009	9.9793	10.0000	0.6
4	50PPBCN	0.043	48.9331	50.0000	1.0
5	100PPBCN	0.088	100.6416	100.0000	
6	250PPBCN	0.219	252.5052	250.0000	
7	500PPBCN	0.433	498.7294	500.0000	-0.3

AS
7/29/21