


LB116602

7471B

INSTRUMENT ID: CV1

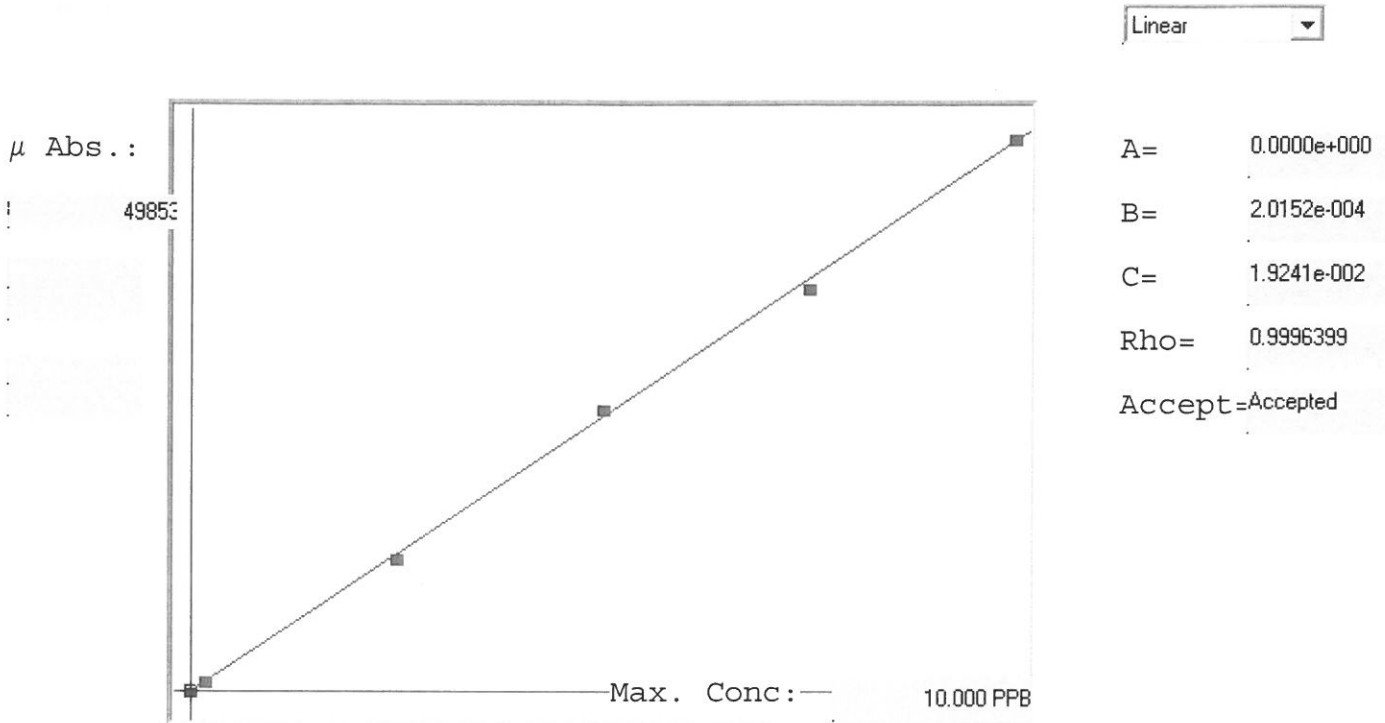

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%1)
0.0	0.000	0.014	0.014	-24	0.000	-24					1
0.2	0.200	0.207	0.007	931	0.0 %	931					3
2.5	2.500	2.441	-0.059	12015	0.0 %	12015					-2
5.0	5.000	5.145	0.145	25435	0.0 %	25435					3
7.5	7.500	7.328	-0.172	36266	0.0 %	36266					1
10.0	10.000	10.066	0.066	49853	0.0 %	49853					0

LB116602 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 01 Oct 2021 10:59:10

Sample ID	Extended ID	μ Abs	Conc.	Std CondMethod	Units	Date	Type	Type
0.0 - 1	SP	-24	-	0.0007471B	PPB	01 Oct 2021 11:00:39	S	Std
0.2 - 1	SP-2	931	-	0.20007471B	PPB	01 Oct 2021 11:02:57	S	Std
2.5 - 1	SP-5	12015	-	2.50007471B	PPB	01 Oct 2021 11:05:14	S	Std
5.0 - 1	SP-5	25435	-	5.00007471B	PPB	01 Oct 2021 11:07:31	S	Std
7.5 - 1	SP-5	36266	-	7.50007471B	PPB	01 Oct 2021 11:09:47	S	Std
10.0 - 1	SP-5	49853	-	10.00007471B	PPB	01 Oct 2021 11:12:06	S	Std
ICV21 - 1	ICV21	19285	3.9056	-7471B	PPB	01 Oct 2021 11:14:44	U	SMPL
ICB21 - 1	ICB21	-214	-0.0239	-7471B	PPB	01 Oct 2021 11:17:01	U	SMPL
CCV60 - 1	CCV60	25659	5.1901	-7471B	PPB	01 Oct 2021 11:21:58	U	SMPL
CCB60 - 1	CCB60	-195	-0.0201	-7471B	PPB	01 Oct 2021 11:24:13	U	SMPL
CRA - 1	CRA	931	0.2069	-7471B	PPB	01 Oct 2021 11:26:29	U	SMPL
HighStd - 1	HighStd	49554	10.0054	-7471B	PPB	01 Oct 2021 11:28:44	U	SMPL
ChkStd - 1	ChkStd	34613	6.9945	-7471B	PPB	01 Oct 2021 11:30:59	U	SMPL
PB139534BL - 1	PBS	-256	-0.0323	-7471B	PPB	01 Oct 2021 11:33:17	U	SMPL
PB139534BS - 1	LCSS	17517	3.5493	-7471B	PPB	01 Oct 2021 11:35:35	U	SMPL
M3990-05 - 1	S-836-K1-SO-1-1.5-092921	1374	0.2961	-7471B	PPB	01 Oct 2021 11:37:51	U	SMPL
M3990-05DUP - 1	S-836-K1-SO-1-1.5-092921DUP	1176	0.2562	-7471B	PPB	01 Oct 2021 11:40:09	U	SMPL
M3990-06 - 1	M3990-05MS	21519	4.3558	-7471B	PPB	01 Oct 2021 11:42:26	U	SMPL
M3990-07 - 1	M3990-05MSD	21627	4.3775	-7471B	PPB	01 Oct 2021 11:44:42	U	SMPL
M3998-01 - 1	MIXED-DEBRIS-1	13306	2.7007	-7471B	PPB	01 Oct 2021 11:46:58	U	SMPL
CCV61 - 1	CCV61	25892	5.2370	-7471B	PPB	01 Oct 2021 11:49:14	U	SMPL
CCB61 - 1	CCB61	-86	0.0019	-7471B	PPB	01 Oct 2021 11:51:29	U	SMPL
M3998-03 - 1	MIXED-DEBRIS-2	7741	1.5792	-7471B	PPB	01 Oct 2021 11:53:44	U	SMPL
M3999-01 - 1	229-342	432397	HIGH	-7471B	PPB	01 Oct 2021 11:56:00	X	
M3999-03 - 1	219	332	0.0861	-7471B	PPB	01 Oct 2021 11:57:48	U	SMPL
M3999-05 - 1	26498	17574	3.5608	-7471B	PPB	01 Oct 2021 12:00:06	U	SMPL
M4005-18 - 1	BU-08-093021	1382	0.2977	-7471B	PPB	01 Oct 2021 12:02:23	U	SMPL
M4007-01 - 1	TR-08-093021	969	0.2145	-7471B	PPB	01 Oct 2021 12:04:39	U	SMPL
M3999-01DLX10 - 1		72056	14.5401	-7471B	PPB	01 Oct 2021 12:06:55	U	SMPL
M3990-05LX5 - 1		-50	0.0092	-7471B	PPB	01 Oct 2021 12:09:12	U	SMPL
M3990-05A - 1		21377	4.3272	-7471B	PPB	01 Oct 2021 12:11:30	U	SMPL
M3999-01DLX20 - 1		32988	6.6670	-7471B	PPB	01 Oct 2021 12:13:46	U	SMPL
CCV62 - 1	CCV62	26936	5.4474	-7471B	PPB	01 Oct 2021 12:16:01	U	SMPL
CCB62 - 1	CCB62	-96	-0.0001	-7471B	PPB	01 Oct 2021 12:18:17	U	SMPL