


LB116617

7471B

INSTRUMENT ID: CV2

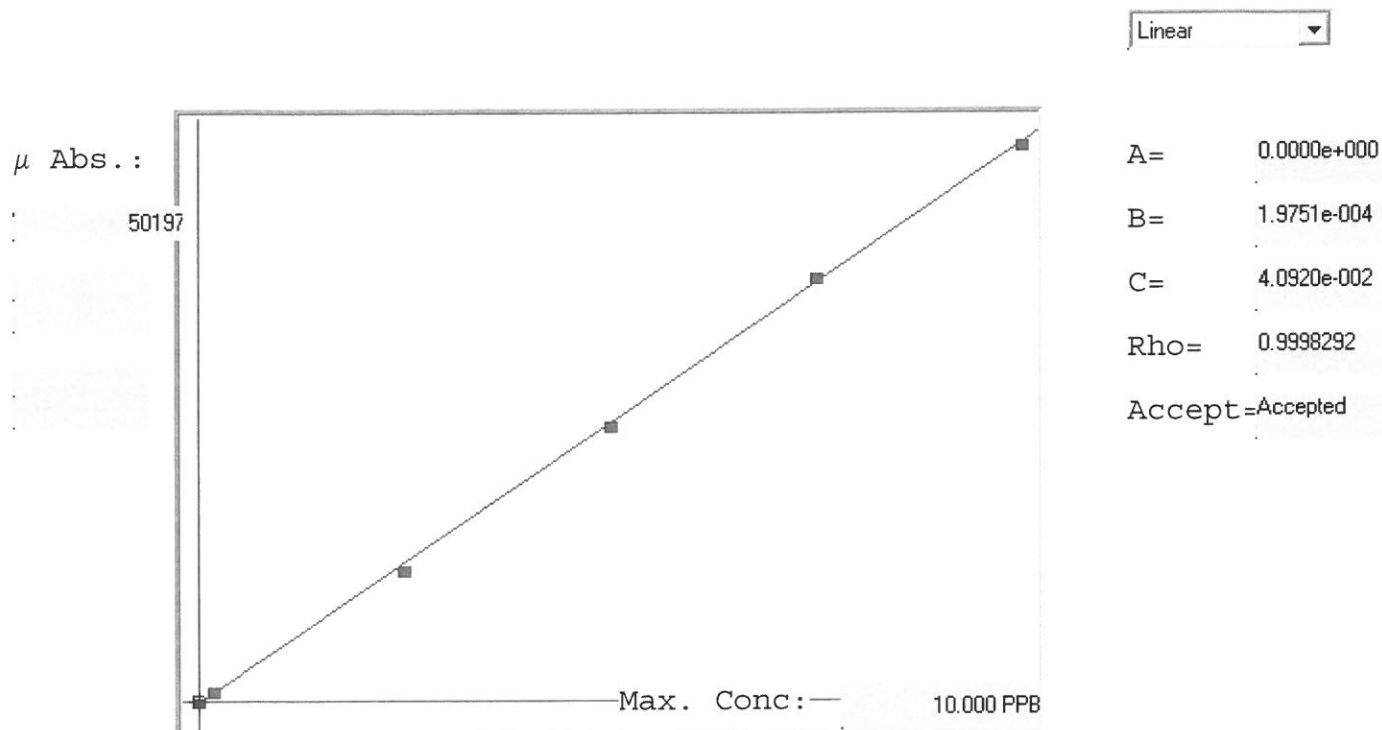

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	0/0/1
0.0	0.000	0.050	0.050	47	0.000	47					
0.2	0.200	0.215	0.015	882	0.0 %	882					
2.5	2.500	2.406	-0.094	11972	0.0 %	11972					
5.0	5.000	4.961	-0.039	24909	0.0 %	24909					
7.5	7.500	7.613	0.113	38336	0.0 %	38336					
10.0	10.000	9.956	-0.044	50197	0.0 %	50197					

LB116617 INSTRUMENT ID : CV1

Method: 7471B	Operator: Admin	Date of Analysis: 02 Oct 2021 14:28:44							
Sample ID	Extended ID	µ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	47	-	0.0000	7471B	PPB	02 Oct 2021 14:32:48	S	Std
0.2 - 1	50.2	882	-	0.2000	7471B	PPB	02 Oct 2021 14:35:05	S	Std
2.5 - 1	52.5	11972	-	2.5000	7471B	PPB	02 Oct 2021 14:37:21	S	Std
5.0 - 1	55	24909	-	5.0000	7471B	PPB	02 Oct 2021 14:39:38	S	Std
7.5 - 1	57.5	38336	-	7.5000	7471B	PPB	02 Oct 2021 14:41:57	S	Std
10.0 - 1	511	50197	-	10.0000	7471B	PPB	02 Oct 2021 14:44:13	S	Std
ICV24 - 1	ICV24	19545	3.9013	-7471B	PPB	PPB	02 Oct 2021 14:47:06	U	SMPL
ICB24 - 1	ICB24	-209	-0.0004	-7471B	PPB	PPB	02 Oct 2021 14:49:20	U	SMPL
CCV76 - 1	CCV76	25227	5.0236	-7471B	PPB	PPB	02 Oct 2021 14:51:36	U	SMPL
CCB76 - 1	CCB76	-224	-0.0033	-7471B	PPB	PPB	02 Oct 2021 14:53:51	U	SMPL
CRA - 1	CRA	798	0.1985	-7471B	PPB	PPB	02 Oct 2021 14:56:07	U	SMPL
HighStd - 1	HighStd	50155	9.9472	-7471B	PPB	PPB	02 Oct 2021 14:58:22	U	SMPL
ChkStd - 1	ChkStd	35989	7.1492	-7471B	PPB	PPB	02 Oct 2021 15:00:37	U	SMPL
PB139566BL - 1	PBS	-286	-0.0156	-7471B	PPB	PPB	02 Oct 2021 15:02:55	U	SMPL
PB139566BS - 1	LCSS	19132	3.8198	-7471B	PPB	PPB	02 Oct 2021 15:05:13	U	SMPL
M4033-01 - 1	SAND-BLAST-DRUMS-1-3	2253	0.4859	-7471B	PPB	PPB	02 Oct 2021 15:07:29	U	SMPL
M4035-02 - 1	12000	2478	0.5304	-7471B	PPB	PPB	02 Oct 2021 15:09:47	U	SMPL
M4035-04 - 1	286	2075	0.4508	-7471B	PPB	PPB	02 Oct 2021 15:12:04	U	SMPL
M4035-06 - 1	205	1592	0.3554	-7471B	PPB	PPB	02 Oct 2021 15:14:21	U	SMPL
M4035-08 - 1	369	2641	0.5626	-7471B	PPB	PPB	02 Oct 2021 15:16:36	U	SMPL
CCV77 - 1	CCV77	25236	5.0254	-7471B	PPB	PPB	02 Oct 2021 15:18:51	U	SMPL
CCB77 - 1	CCB77	-100	0.0212	-7471B	PPB	PPB	02 Oct 2021 15:21:07	U	SMPL
M4035-10 - 1	213	1555	0.3481	-7471B	PPB	PPB	02 Oct 2021 15:23:22	U	SMPL
M4035-12 - 1	218	1586	0.3542	-7471B	PPB	PPB	02 Oct 2021 15:25:38	U	SMPL
M4036-02 - 1	211	1679	0.3725	-7471B	PPB	PPB	02 Oct 2021 15:27:53	U	SMPL
M4037-01 - 1	HD-01-100121	918	0.2222	-7471B	PPB	PPB	02 Oct 2021 15:30:09	U	SMPL
M4039-01 - 1	TP-1	8712	1.7617	-7471B	PPB	PPB	02 Oct 2021 15:32:25	U	SMPL
M4039-04 - 1	TP-2	2358	0.5067	-7471B	PPB	PPB	02 Oct 2021 15:34:41	U	SMPL
M4039-04DUP - 1	TP-2DUP	1963	0.4286	-7471B	PPB	PPB	02 Oct 2021 15:36:57	U	SMPL
M4039-04MS - 1	TP-2MS	22056	4.3973	-7471B	PPB	PPB	02 Oct 2021 15:39:14	U	SMPL
M4039-04MSD - 1	TP-2MSD	21908	4.3681	-7471B	PPB	PPB	02 Oct 2021 15:41:31	U	SMPL
PB139567BL - 1	PBS	-61	0.0289	-7471B	PPB	PPB	02 Oct 2021 15:43:47	U	SMPL
CCV78 - 1	CCV78	25424	5.0625	-7471B	PPB	PPB	02 Oct 2021 15:46:02	U	SMPL
CCB78 - 1	CCB78	-65	0.0281	-7471B	PPB	PPB	02 Oct 2021 15:48:18	U	SMPL
PB139567BS - 1	LCSS	19559	3.9041	-7471B	PPB	PPB	02 Oct 2021 15:50:33	U	SMPL
M4032-01 - 1	NB-08-100121	1444	0.3261	-7471B	PPB	PPB	02 Oct 2021 15:52:49	U	SMPL
M4032-01DUP - 1	NB-08-100121DUP	1727	0.3820	-7471B	PPB	PPB	02 Oct 2021 15:55:05	U	SMPL
M4032-01MS - 1	NB-08-100121MS	21974	4.3811	-7471B	PPB	PPB	02 Oct 2021 15:57:20	U	SMPL
M4032-01MSD - 1	NB-08-100121MSD	21327	4.2533	-7471B	PPB	PPB	02 Oct 2021 15:59:35	U	SMPL
M4042-01 - 1	EO-01-100121	10812	2.1764	-7471B	PPB	PPB	02 Oct 2021 16:01:51	U	SMPL
M4042-03 - 1	EO-02-100121	7270	1.4768	-7471B	PPB	PPB	02 Oct 2021 16:04:08	U	SMPL
M4042-05 - 1	EO-03-100121	2154	0.4664	-7471B	PPB	PPB	02 Oct 2021 16:06:25	U	SMPL
M4043-01 - 1	HR-03-100121	2030	0.4419	-7471B	PPB	PPB	02 Oct 2021 16:08:42	U	SMPL
M4043-03 - 1	HR-04-100121	9015	1.8215	-7471B	PPB	PPB	02 Oct 2021 16:10:58	U	SMPL
CCV79 - 1	CCV79	25567	5.0908	-7471B	PPB	PPB	02 Oct 2021 16:13:14	U	SMPL
CCB79 - 1	CCB79	-18	0.0374	-7471B	PPB	PPB	02 Oct 2021 16:15:29	U	SMPL
M4046-01 - 1	TP-1-(1.0-1.5)	4545	0.9386	-7471B	PPB	PPB	02 Oct 2021 16:17:45	U	SMPL
M4046-03 - 1	TP-1-(3.0-3.5)	1654	0.3676	-7471B	PPB	PPB	02 Oct 2021 16:20:00	U	SMPL
M4046-04 - 1	TP-1-(4.5-5.0)	5113	1.0508	-7471B	PPB	PPB	02 Oct 2021 16:22:16	U	SMPL
M4047-01 - 1	149-ENV-1-GRAB	20878	4.1646	-7471B	PPB	PPB	02 Oct 2021 16:24:31	U	SMPL
M4047-03 - 1	149-ENV-1-COMPOSITE	21355	4.2588	-7471B	PPB	PPB	02 Oct 2021 16:26:46	U	SMPL
M4039-04LX5 - 1		364	0.1128	-7471B	PPB	PPB	02 Oct 2021 16:29:03	U	SMPL
M4039-04A - 1		22099	4.4058	-7471B	PPB	PPB	02 Oct 2021 16:31:19	U	SMPL
M4032-01LX5 - 1		187	0.0779	-7471B	PPB	PPB	02 Oct 2021 16:33:36	U	SMPL
M4032-01A - 1		21917	4.3698	-7471B	PPB	PPB	02 Oct 2021 16:35:53	U	SMPL
CCV80 - 1	CCV80	26116	5.1992	-7471B	PPB	PPB	02 Oct 2021 16:38:09	U	SMPL
CCB80 - 1	CCB80	-59	0.0293	-7471B	PPB	PPB	02 Oct 2021 16:40:24	U	SMPL