


LB 116715

245.1

INSTRUMENT ID: CV1

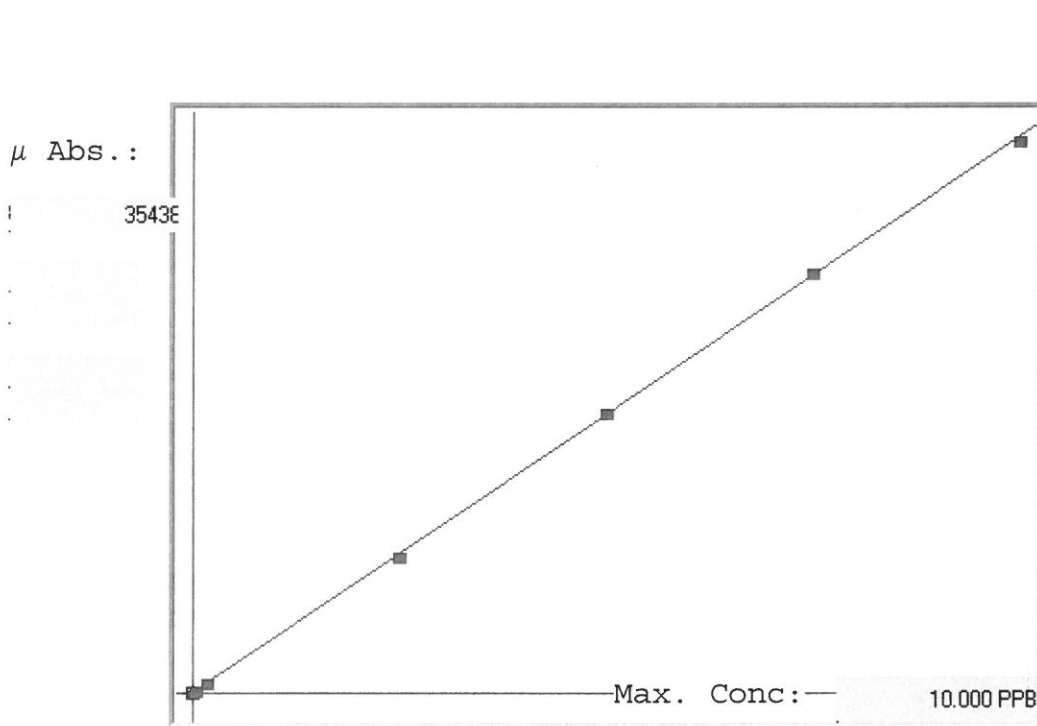

Linear

A= 0.0000e+000

B= 2.8049e-004

C= -6.1909e-004

Rho= 0.9999482

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%
0.0	0.000	-0.006	-0.006	-20	0.000	-20					-2
0.05	0.050	0.049	-0.001	176	0.0 %	176	0				-3
0.2	0.200	0.195	-0.005	699	0.0 %	699					-1
2.5	2.500	2.472	-0.028	8815	0.0 %	8815					-1
5.0	5.000	5.035	0.035	17954	0.0 %	17954					-1
7.5	7.500	7.565	0.065	26973	0.0 %	26973					-1
10.0	10.000	9.940	-0.060	35438	0.0 %	35438					0

LB116715 INSTRUMENT ID : CV1

Method: 245.1

Operator: Admin

Date of Analysis: 07 Oct 2021 12:03:49

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	-20	-	0.0000	245.1	PPB	07 Oct 2021 12:13:09	S	Std
0.05 - 1	50.05	176	-	0.0500	245.1	PPB	07 Oct 2021 12:15:27	S	Std
0.2 - 1	50.2	699	-	0.2000	245.1	PPB	07 Oct 2021 12:17:44	S	Std
2.5 - 1	52.5	8815	-	2.5000	245.1	PPB	07 Oct 2021 12:20:01	S	Std
5.0 - 1	55	17954	-	5.0000	245.1	PPB	07 Oct 2021 12:22:17	S	Std
7.5 - 1	57.5	26973	-	7.5000	245.1	PPB	07 Oct 2021 12:24:33	S	Std
10.0 - 1	510	35438	-	10.0000	245.1	PPB	07 Oct 2021 12:26:50	S	Std
ICV33 - 1	ICV33	13574	3.8068	-245.1		PPB	07 Oct 2021 12:29:36	U	SMPL
ICB33 - 1	ICB33	-138	-0.0393	-245.1		PPB	07 Oct 2021 12:31:51	U	SMPL
CCV12 - 1	CCV12	17991	5.0458	-245.1		PPB	07 Oct 2021 12:36:50	U	SMPL
CCB12 - 1	CCB12	-153	-0.0435	-245.1		PPB	07 Oct 2021 12:39:05	U	SMPL
CRA - 1	CRA	153	0.0423	-245.1		PPB	07 Oct 2021 12:44:07	U	SMPL
HighStd - 1	HighStd	35032	9.8257	-245.1		PPB	07 Oct 2021 12:46:22	U	SMPL
ChkStd - 1	ChkStd	25685	7.2039	-245.1		PPB	07 Oct 2021 12:48:37	U	SMPL
PB139710BL - 1	PBW	-229	-0.0649	-245.1		PPB	07 Oct 2021 12:50:55	U	SMPL
PB139710BS - 1	LCSW	14330	4.0189	-245.1		PPB	07 Oct 2021 12:53:13	U	SMPL
M4049-01 - 1	MW-1	616	0.1722	-245.1		PPB	07 Oct 2021 13:00:22	U	SMPL
M4049-01DUP - 1	MW-1DUP	513	0.1433	-245.1		PPB	07 Oct 2021 13:02:38	U	SMPL
M4049-01MS - 1	MW-1MS	16203	4.5442	-245.1		PPB	07 Oct 2021 13:04:55	U	SMPL
M4049-01MSD - 1	MW-1MSD	16394	4.5978	-245.1		PPB	07 Oct 2021 13:07:12	U	SMPL
M4100-02 - 1	COMP	198	0.0549	-245.1		PPB	07 Oct 2021 13:09:27	U	SMPL
CCV13 - 1	CCV13	17689	4.9611	-245.1		PPB	07 Oct 2021 13:11:42	U	SMPL
CCB13 - 1	CCB13	-59	-0.0172	-245.1		PPB	07 Oct 2021 13:13:58	U	SMPL
M4104-01 - 1	55TH-ST-33	24	0.0061	-245.1		PPB	07 Oct 2021 13:16:14	U	SMPL
M4049-01LX5 - 1		300	0.0835	-245.1		PPB	07 Oct 2021 13:18:30	U	SMPL
M4049-01A - 1		15511	4.3501	-245.1		PPB	07 Oct 2021 13:20:45	U	SMPL
CCV14 - 1	CCV14	17833	5.0014	-245.1		PPB	07 Oct 2021 13:23:01	U	SMPL
CCB14 - 1	CCB14	-19	-0.0059	-245.1		PPB	07 Oct 2021 13:25:16	U	SMPL