


LB116745

7471B

INSTRUMENT ID: CV2

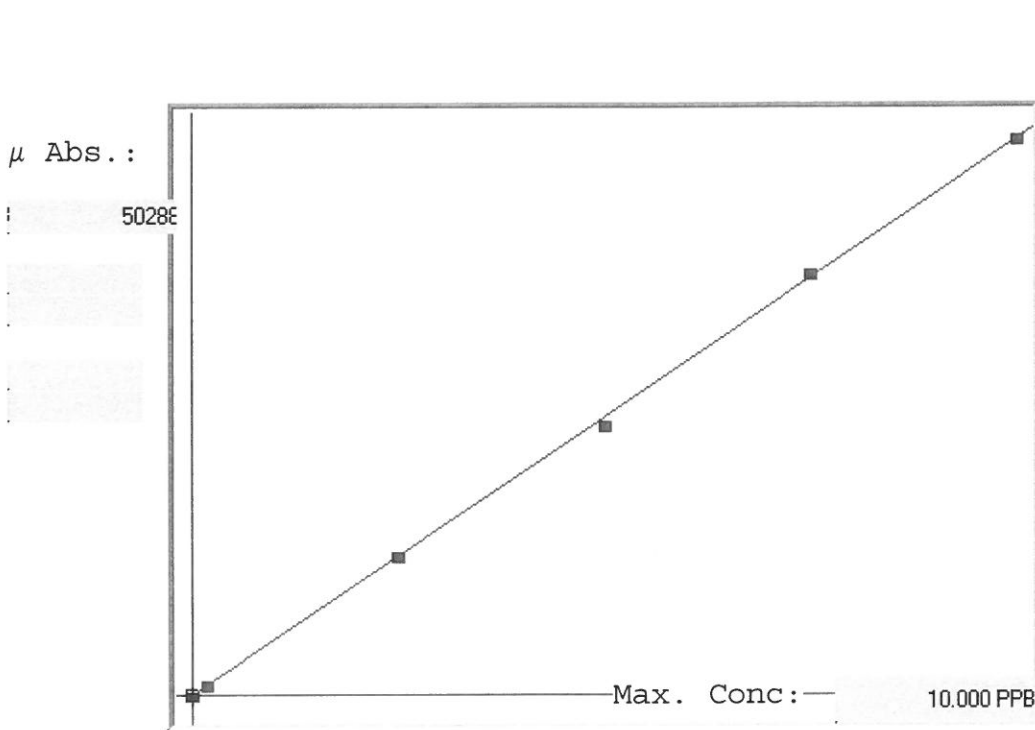

Linear

A= 0.0000e+000

B= 1.9849e-004

C= 1.4873e-002

Rho= 0.9998513

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	0.016	0.016	6	0.000	6					2
0.2	0.200	0.214	0.014	1004	0.0 %	1004					7
2.5	2.500	2.523	0.023	12638	0.0 %	12638					1
5.0	5.000	4.870	-0.130	24460	0.0 %	24460					-3
7.5	7.500	7.580	0.080	38112	0.0 %	38112					1
10.0	10.000	9.997	-0.003	50288	0.0 %	50288					0

LB116745 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 08 Oct 2021 12:59:51

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	6	-	0.0000	7471B	PPB	08 Oct 2021 13:00:55	S	Std
0.2 - 1	502	1004	-	0.2000	7471B	PPB	08 Oct 2021 13:03:12	S	Std
2.5 - 1	52.5	12638	-	2.5000	7471B	PPB	08 Oct 2021 13:05:29	S	Std
5.0 - 1	55	24460	-	5.0000	7471B	PPB	08 Oct 2021 13:07:46	S	Std
7.5 - 1	59.5	38112	-	7.5000	7471B	PPB	08 Oct 2021 13:10:03	S	Std
10.0 - 1	570	50288	-	10.0000	7471B	PPB	08 Oct 2021 13:12:20	S	Std
ICV36 - 1	ICV36	19711	3.9273	-	7471B	PPB	08 Oct 2021 13:15:02	U	SMPL
ICB36 - 1	ICB36	-132	-0.0113	-	7471B	PPB	08 Oct 2021 13:17:17	U	SMPL
CCV26 - 1	CCV26	24298	4.8378	-	7471B	PPB	08 Oct 2021 13:19:33	U	SMPL
CCB26 - 1	CCB26	-139	-0.0127	-	7471B	PPB	08 Oct 2021 13:21:48	U	SMPL
CRA - 1	CRA	976	0.2086	-	7471B	PPB	08 Oct 2021 13:24:04	U	SMPL
HighStd - 1	HighStd	50294	9.9978	-	7471B	PPB	08 Oct 2021 13:26:19	U	SMPL
ChkStd - 1	ChkStd	35784	7.1177	-	7471B	PPB	08 Oct 2021 13:28:34	U	SMPL
PB139748BL - 1	PBS	-214	-0.0276	-	7471B	PPB	08 Oct 2021 13:30:52	U	SMPL
PB139748BS - 1	LCSS	19544	3.8942	-	7471B	PPB	08 Oct 2021 13:36:52	U	SMPL
M4127-01 - 1	CHRT-27080	6621	1.3291	-	7471B	PPB	08 Oct 2021 13:39:08	U	SMPL
M4127-03 - 1	CHRT-27051	28556	5.6830	-	7471B	PPB	08 Oct 2021 13:41:24	U	SMPL
M4127-05 - 1	CHRT-20426	3440	0.6977	-	7471B	PPB	08 Oct 2021 13:43:41	U	SMPL
M4127-08 - 1	CHRT-26644	6072	1.2201	-	7471B	PPB	08 Oct 2021 13:45:58	U	SMPL
M4129-01 - 1	OK-02-100721	1318	0.2765	-	7471B	PPB	08 Oct 2021 13:48:13	U	SMPL
CCV27 - 1	CCV27	24500	4.8779	-	7471B	PPB	08 Oct 2021 13:50:28	U	SMPL
CCB27 - 1	CCB27	-63	0.0024	-	7471B	PPB	08 Oct 2021 13:52:44	U	SMPL
M4136-01 - 1	PSC124055	4645	0.9369	-	7471B	PPB	08 Oct 2021 13:55:00	U	SMPL
M4136-03 - 1	PSC124027	1498	0.3122	-	7471B	PPB	08 Oct 2021 13:57:15	U	SMPL
M4136-05 - 1	PSC124042	6014	1.2086	-	7471B	PPB	08 Oct 2021 13:59:30	U	SMPL
M4142-01 - 1	ETGI-330	10693	2.1373	-	7471B	PPB	08 Oct 2021 14:01:46	U	SMPL
M4142-01DUP - 1	ETGI-330DUP	11641	2.3255	-	7471B	PPB	08 Oct 2021 14:04:02	U	SMPL
M4142-01MS - 1	ETGI-330MS	28731	5.7177	-	7471B	PPB	08 Oct 2021 14:08:56	U	SMPL
M4142-01MSD - 1	ETGI-330MSD	27982	5.5691	-	7471B	PPB	08 Oct 2021 14:11:12	U	SMPL
M4142-01LX5 - 1		2062	0.4242	-	7471B	PPB	08 Oct 2021 14:13:30	U	SMPL
M4142-01A - 1		31139	6.1957	-	7471B	PPB	08 Oct 2021 14:15:48	U	SMPL
M4131-04DLX2 - 1		37276	7.4138	-	7471B	PPB	08 Oct 2021 14:21:19	U	SMPL
CCV28 - 1	CCV28	24994	4.9760	-	7471B	PPB	08 Oct 2021 14:23:35	U	SMPL
CCB28 - 1	CCB28	-84	-0.0018	-	7471B	PPB	08 Oct 2021 14:25:51	U	SMPL