


LB116833

7470A

INSTRUMENT ID: CV2

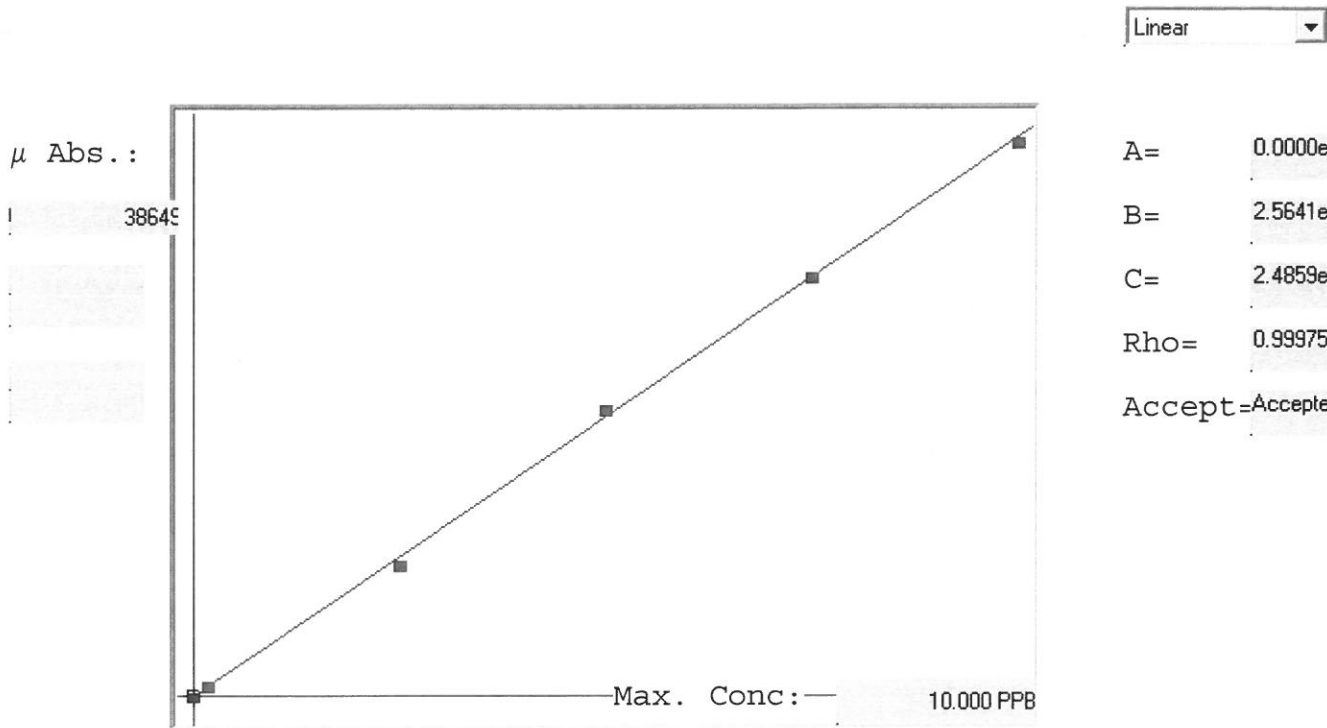

A= 0.0000e+000

B= 2.5641e-004

C= 2.4859e-002

Rho= 0.9997510

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	0.023	0.023	-8	0.000	-8					1
0.2	0.200	0.197	-0.003	672	0.0 %	672					-2
2.5	2.500	2.376	-0.124	9168	0.0 %	9168					-5
5.0	5.000	5.140	0.140	19948	0.0 %	19948					3
7.5	7.500	7.530	0.030	29271	0.0 %	29271					0
10.0	10.000	9.935	-0.065	38649	0.0 %	38649					-1

LB116833 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 14 Oct 2021 12:33:53

Sample ID	Extended ID	μ Abs.	Conc.	Std. Conc.	Method	Units	Date	Type	Type
0.0 - 1	5.5	-8	-	0.00007470A	PPB		14 Oct 2021	12:36:22	S Std
0.2 - 1	56.2	672	-	0.20007470A	PPB		14 Oct 2021	12:38:39	S Std
2.5 - 1	52.5	9168	-	2.50007470A	PPB		14 Oct 2021	12:40:57	S Std
5.0 - 1	55	19948	-	5.00007470A	PPB		14 Oct 2021	12:43:14	S Std
7.5 - 1	59.5	29271	-	7.50007470A	PPB		14 Oct 2021	12:45:30	S Std
10.0 - 1	510	38649	-	10.00007470A	PPB		14 Oct 2021	12:50:19	S Std
ICV43 - 1	ICV43	15605	4.0261	-7470A	PPB		14 Oct 2021	12:58:17	U SMPL
ICB43 - 1	ICB43	-151	-0.0139	-7470A	PPB		14 Oct 2021	13:00:32	U SMPL
CCV55 - 1	CCV55	18902	4.8714	-7470A	PPB		14 Oct 2021	13:02:47	U SMPL
CCB55 - 1	CCB55	-144	-0.0121	-7470A	PPB		14 Oct 2021	13:05:02	U SMPL
CRA - 1	CRA	586	0.1751	-7470A	PPB		14 Oct 2021	13:07:18	U SMPL
HighStd - 1	HighStd	39050	10.0375	-7470A	PPB		14 Oct 2021	13:09:33	U SMPL
ChkStd - 1	ChkStd	26348	6.7806	-7470A	PPB		14 Oct 2021	13:11:49	U SMPL
PB139896BL - 1	PBW	-242	-0.0372	-7470A	PPB		14 Oct 2021	13:14:06	U SMPL
PB139896BS - 1	LCSW	13768	3.5551	-7470A	PPB		14 Oct 2021	13:16:23	U SMPL
M4189-01 - 1	345-3	3061	0.8097	-7470A	PPB		14 Oct 2021	13:18:39	U SMPL
M4190-01 - 1	P287-DITCH	564	0.1695	-7470A	PPB		14 Oct 2021	13:23:26	U SMPL
M4190-01DUP - 1	P287-DITCHDUP	391	0.1251	-7470A	PPB		14 Oct 2021	13:28:36	U SMPL
M4190-01MS - 1	P287-DITCHMS	13450	3.4735	-7470A	PPB		14 Oct 2021	13:30:53	U SMPL
M4190-01MSD - 1	P287-DITCHMSD	13275	3.4286	-7470A	PPB		14 Oct 2021	13:33:09	U SMPL
CCV56 - 1	CCV56	19326	4.9802	-7470A	PPB		14 Oct 2021	13:35:25	U SMPL
CCB56 - 1	CCB56	-81	0.0041	-7470A	PPB		14 Oct 2021	13:37:41	U SMPL
M4190-02 - 1	P287-DITCH	44	0.0361	-7470A	PPB		14 Oct 2021	13:43:16	U SMPL
M4190-03 - 1	SW-RR-03-(SA)	-11	0.0220	-7470A	PPB		14 Oct 2021	13:45:31	U SMPL
M4190-04 - 1	SW-RR-03-(SA)	-16	0.0208	-7470A	PPB		14 Oct 2021	13:47:46	U SMPL
M4190-05 - 1	SW-RR-01-(2.0)	-13	0.0215	-7470A	PPB		14 Oct 2021	13:50:01	U SMPL
M4190-06 - 1	SW-RR-01-(2.0)	26	0.0315	-7470A	PPB		14 Oct 2021	13:52:18	U SMPL
PB139901BL - 1	PBW	8	0.0269	-7470A	PPB		14 Oct 2021	13:54:34	U SMPL
PB139901BS - 1	LCSW	13860	3.5786	-7470A	PPB		14 Oct 2021	13:56:50	U SMPL
M4180-02 - 1	NYPD-69TH-WC-1	3	0.0256	-7470A	PPB		14 Oct 2021	13:59:07	U SMPL
M4180-02DUP - 1	NYPD-69TH-WC-1DUP	11	0.0277	-7470A	PPB		14 Oct 2021	14:01:24	U SMPL
M4180-02MS - 1	NYPD-69TH-WC-1MS	16238	4.1884	-7470A	PPB		14 Oct 2021	14:03:40	U SMPL
CCV57 - 1	CCV57	19158	4.9371	-7470A	PPB		14 Oct 2021	14:05:56	U SMPL
CCB57 - 1	CCB57	-125	-0.0072	-7470A	PPB		14 Oct 2021	14:08:11	U SMPL
PB139902BL - 1	PBW	-144	-0.0121	-7470A	PPB		14 Oct 2021	14:12:43	U SMPL
M4195-02 - 1	HAR-SOILPILE	-65	0.0082	-7470A	PPB		14 Oct 2021	14:17:16	U SMPL
M4202-01 - 1	CS-1-DEPTH-SOILPILE-BOTTOM	0	0.0249	-7470A	PPB		14 Oct 2021	14:19:32	U SMPL
M4202-01DUP - 1	CS-1-DEPTH-SOILPILE-BOTTOMDUP	1	0.0251	-7470A	PPB		14 Oct 2021	14:21:48	U SMPL
M4202-01MS - 1	CS-1-DEPTH-SOILPILE-BOTTOMMS	13880	3.5838	-7470A	PPB		14 Oct 2021	14:33:17	U SMPL
M4202-01MSD - 1	CS-1-DEPTH-SOILPILE-BOTTOMMSD	15114	3.9002	-7470A	PPB		14 Oct 2021	14:35:34	U SMPL
PB139901TB - 1	PB139848TB	-115	-0.0046	-7470A	PPB		14 Oct 2021	14:37:51	U SMPL
PB139902TB - 1	PB139881TB	-28	0.0177	-7470A	PPB		14 Oct 2021	14:40:07	U SMPL
CCV58 - 1	CCV58	17865	4.6055	-7470A	PPB		14 Oct 2021	14:42:22	U SMPL
CCB58 - 1	CCB58	-128	-0.0080	-7470A	PPB		14 Oct 2021	14:44:38	U SMPL
M4190-01LX5 - 1		82	0.0459	-7470A	PPB		14 Oct 2021	14:46:54	U SMPL
M4190-01A - 1		14018	3.6192	-7470A	PPB		14 Oct 2021	14:49:10	U SMPL
M4180-02LX5 - 1		-75	0.0056	-7470A	PPB		14 Oct 2021	14:51:25	U SMPL
M4180-02A - 1		14112	3.6433	-7470A	PPB		14 Oct 2021	14:53:41	U SMPL
M4202-01LX5 - 1		-35	0.0159	-7470A	PPB		14 Oct 2021	14:55:56	U SMPL
M4202-01A - 1		13850	3.5761	-7470A	PPB		14 Oct 2021	14:58:13	U SMPL
M4180-02MSD - 1	NYPD-69TH-WC-1MSD	15196	3.9212	-7470A	PPB		14 Oct 2021	15:02:48	U SMPL
PB139902BS - 1	LCSW	15149	3.9092	-7470A	PPB		14 Oct 2021	15:05:04	U SMPL
CCV59 - 1	CCV59	19777	5.0958	-7470A	PPB		14 Oct 2021	15:07:21	U SMPL
CCB59 - 1	CCB59	-138	-0.0105	-7470A	PPB		14 Oct 2021	15:09:37	U SMPL