

Clear table


Clear table

Clear table

Instrument ID: IC-2									
Analyst: AP				Method: 300 / 9056A					
ident	concentration F-	concentration CL-	concentration on NO2	concentration on BR-	concentration on NO3	concentration on HPO4	concentration on SO4	file name	date time
ident	True Value F-	True Value CL-	True Value NO2	True Value BR-	True Value NO3	True Value HPO4	True Value SO4		Initial wt/ Final Vol
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2021-10-11_	10/11/21 8:44
STD2	0.4300	0.6780	0.6690	2.2590	0.5740	0.8870	3.5680	2021-10-11_	10/11/21 9:18
STD3	0.8200	1.1940	1.1860	4.0070	1.0020	2.0340	6.0080	2021-10-11_	10/11/21 9:46
STD4	0.9190	1.4550	1.4640	4.8490	1.2160	2.3710	7.2560	2021-10-11_	10/11/21 10:14
STD5	1.9910	2.9530	2.9660	9.8230	2.4380	5.2410	14.5130	2021-10-11_	10/11/21 10:42
STD6	4.2170	5.9970	5.9890	19.9420	4.9810	10.2720	29.8810	2021-10-11_	10/11/21 11:10
STD7	4.8230	7.5230	7.5250	25.1200	6.2890	12.1950	37.7730	2021-10-11_	10/11/21 11:38
ident	True Value F-	True Value CL-	True Value NO2	True Value BR-	True Value NO3	True Value HPO4	True Value SO4		
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000		AP/MA
STD2	0.4000	0.6000	0.6000	2.0000	0.5000	1.0000	3.0000		AP/MA
STD3	0.8000	1.2000	1.2000	4.0000	1.0000	2.0000	6.0000		AP/MA
STD4	1.0000	1.5000	1.5000	5.0000	1.2500	2.5000	7.5000		AP/MA
STD5	2.0000	3.0000	3.0000	10.0000	2.5000	5.0000	15.0000		AP/MA
STD6	4.0000	6.0000	6.0000	20.0000	5.0000	10.0000	30.0000		AP/MA
STD7	5.0000	7.5000	7.5000	25.0000	6.2500	12.5000	37.5000		AP/MA
ident	Relative Error F-	Relative Error CL-	Relative Error NO2	Relative Error BR-	Relative Error NO3	Relative Error HPO4	Relative Error SO4		
STD1									
STD2	7.5000	13.0000	11.5000	12.9500	14.8000	-11.3000	18.9333		
STD3	2.5000	-0.5000	-1.1667	0.1750	0.2000	1.7000	0.1333		
STD4	-8.1000	-3.0000	-2.4000	-3.0200	-2.7200	-5.1600	-3.2533		
STD5	-0.4500	-1.5667	-1.1333	-1.7700	-2.4800	4.8200	-3.2467		
STD6	5.4250	-0.0500	-0.1833	-0.2900	-0.3800	2.7200	-0.3967		
STD7	-3.5400	0.3067	0.3333	0.4800	0.6240	-2.4400	0.7280		

CALIBRATION OF COMPONENT F-

Method: AnionsIC2-101121.mtw
 Equation: $Q = 0.0744588 \cdot A + 1.6749$
 RSD: 6.687 %
 Correlation coefficient: 0.997560

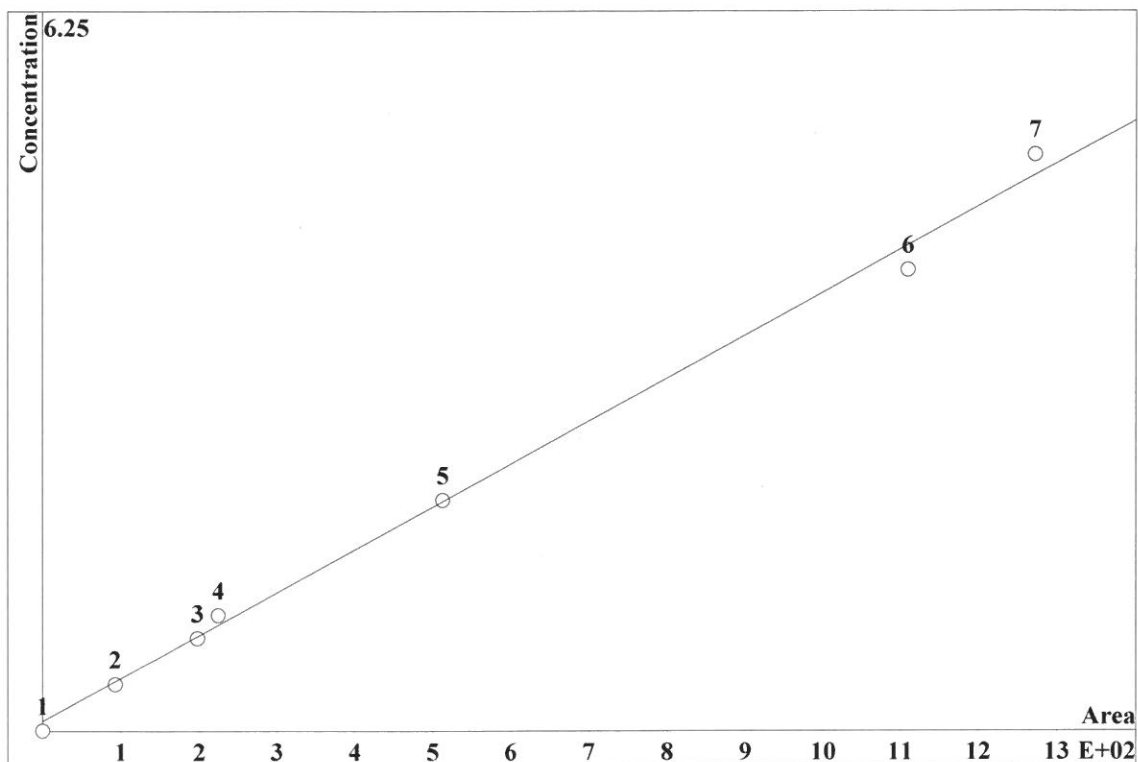

K3 = 0 K2 = 0 K1 = 0.0744588 K0 = 1.6749

Base: Area

Ref.channel: chl

ISTD:


Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used File
1	0	0	0	0	0	0
2	1.78	92.91	0.4	20	5.681	
3	3.828	197.9	0.8	20	5.681	
4	4.665	224.2	1	20	5.681	
5	11.97	512.3	2	20	5.681	
6	24.28	1110	4	20	5.681	
7	29.23	1273	5	20	5.681	

CALIBRATION OF COMPONENT CL-

Method: AnionsIC2-101121.mtw
 Equation: $Q = 0.110027 \cdot A + 3.0598$
 RSD: 1.585 %
 Correlation coefficient: 0.999863

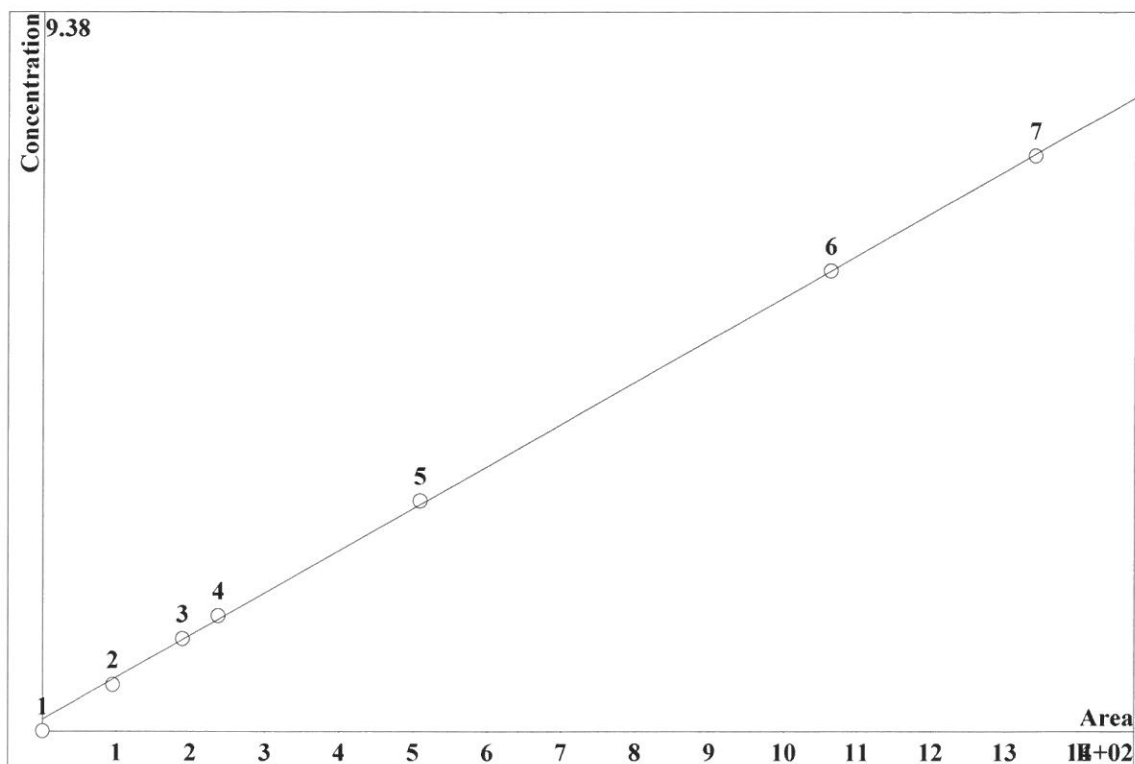

K3 = 0 K2 = 0 K1 = 0.110027 K0 = 3.0598

Base: Area

Ref.channel: ch1

ISTD:


Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used File
1		0	0	0	0	0
2	6.9	95.4	0.6	20	8.597	
3	13.49	189.3	1.2	20	8.597	
4	17.36	236.6	1.5	20	8.597	
5	37.9	508.9	3	20	8.597	
6	80.05	1062	6	20	8.597	
7	102.5	1340	7.5	20	8.597	

CALIBRATION OF COMPONENT NO2

Method: AnionsIC2-101121.mtw
 Equation: $Q = 0.0487979 \cdot A + 3.14089$
 RSD: 1.366 %
 Correlation coefficient: 0.999898

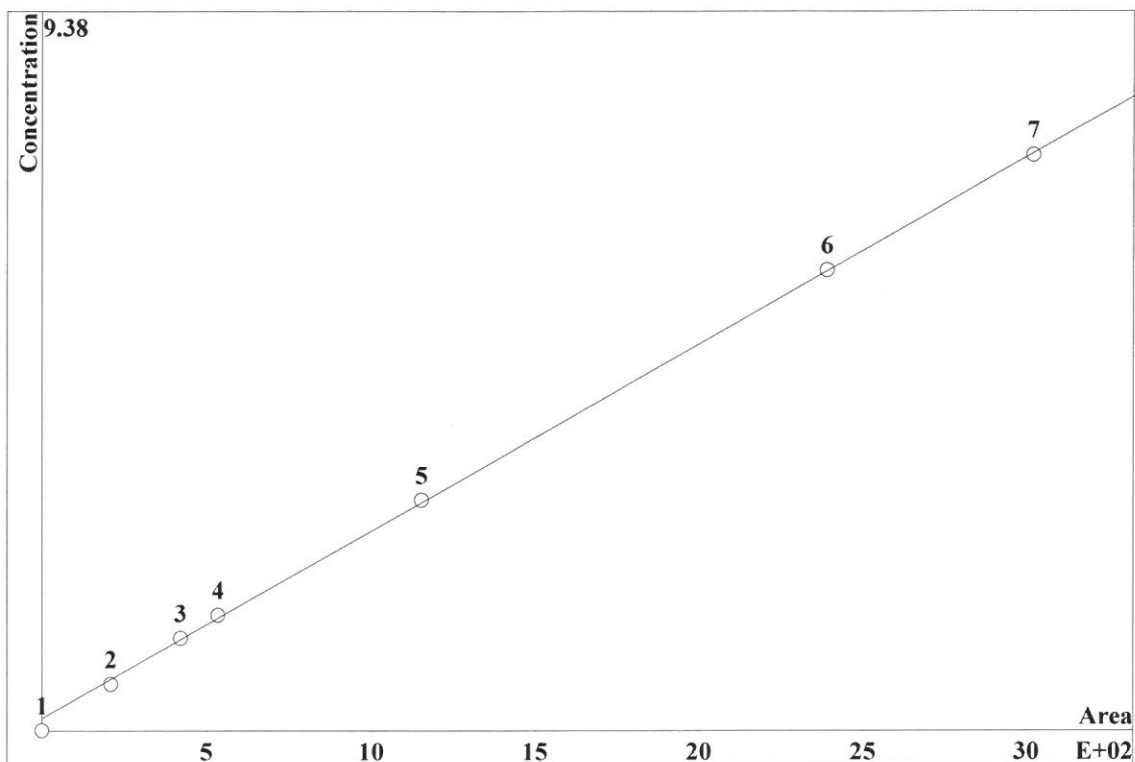

K3 = 0 K2 = 0 K1 = 0.0487979 K0 = 3.14089

Base: Area

Ref.channel: chl

ISTD:


Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used File
1	0	0	0	0	0	0
2	12.43	209.9	0.6	20	10.39	
3	24.79	421.8	1.2	20	10.39	
4	32.09	535.8	1.5	20	10.39	
5	67.48	1151	3	20	10.39	
6	137.9	2390	6	20	10.39	
7	172	3020	7.5	20	10.39	

CALIBRATION OF COMPONENT BR-

Method: AnionsIC2-101121.mtw
 Equation: $Q = 0.245006 \cdot A + 12.0971$
 RSD: 1.694 %
 Correlation coefficient: 0.999844

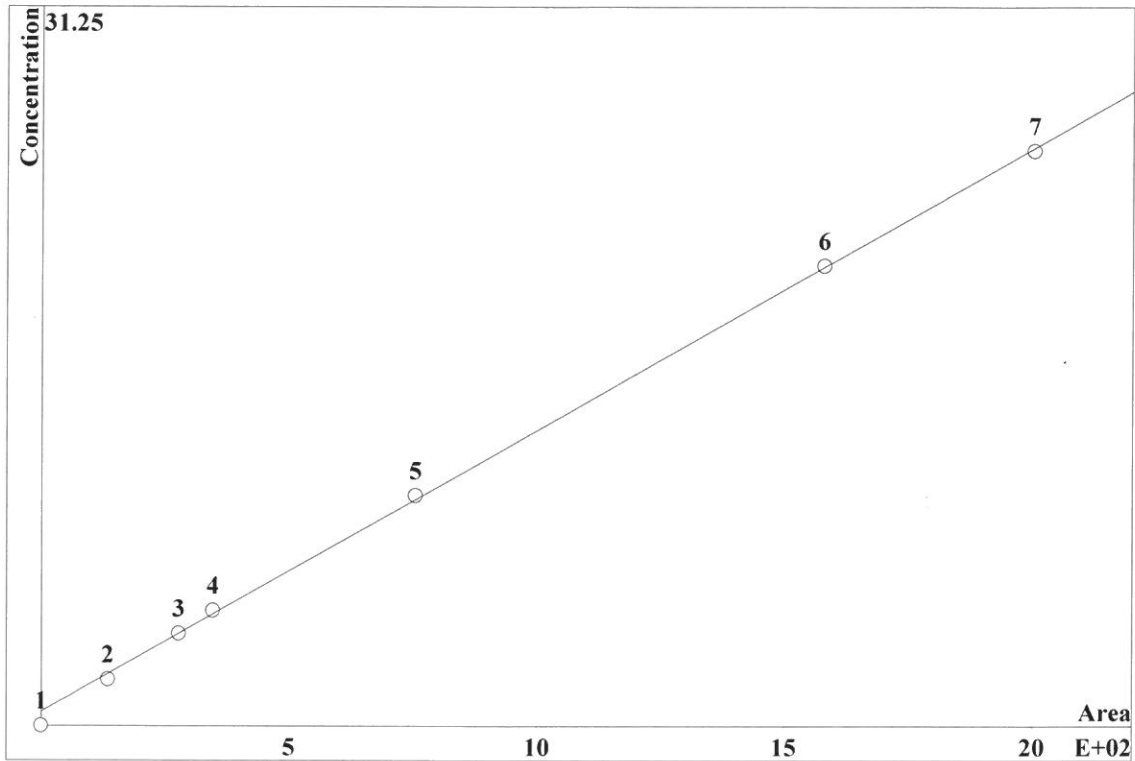


K3 = 0 K2 = 0 K1 = 0.245006 K0 = 12.0971
 Base: Area
 Ref.channel: ch1
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	-0.00298	-0.000298		0	20		13.42
2	7.066	135		2	20		13.42
3	14.35	277.7		4	20		13.42
4	18.53	346.4		5	20		13.42
5	41.08	752.5		10	20		13.42
6	86.24	1579		20	20		13.42
7	109.2	2001		25	20		13.42

CALIBRATION OF COMPONENT NO3

Method: AnionsIC2-101121.mtw
 Equation: $Q = 0.0424654 \cdot A + 3.07921$
 RSD: 2.014 %
 Correlation coefficient: 0.999779

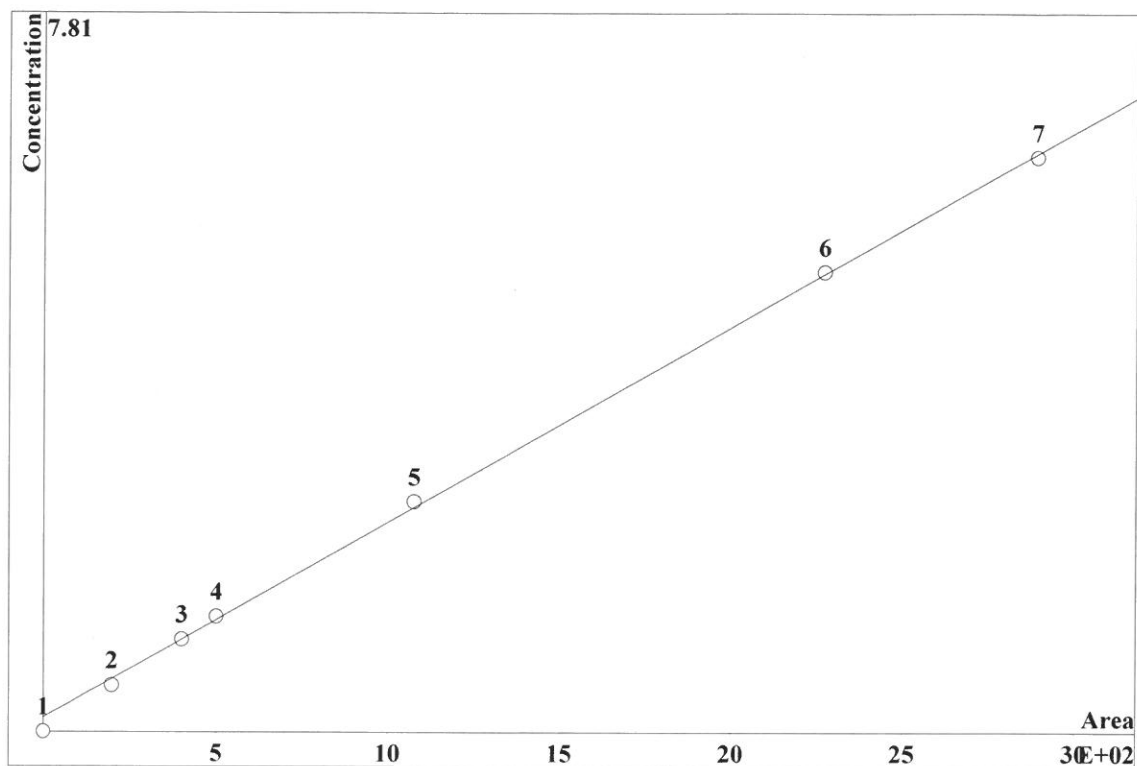

K3 = 0 K2 = 0 K1 = 0.0424654 K0 = 3.07921

Base: Area

Ref.channel: ch1

ISTD:


Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used File
1	0	0	0	0	0	0
2	8.74	197.8	0.5	20	15.44	
3	17.58	399.6	1	20	15.44	
4	22.63	500.2	1.25	20	15.44	
5	49.87	1076	2.5	20	15.44	
6	106.7	2273	5	20	15.44	
7	137.2	2889	6.25	20	15.44	

CALIBRATION OF COMPONENT HPO4

Method: AnionsIC2-101121.mtw
 Equation: $Q = 0.0894674 \cdot A - 6.00166$
 RSD: 4.593 %
 Correlation coefficient: 0.998849

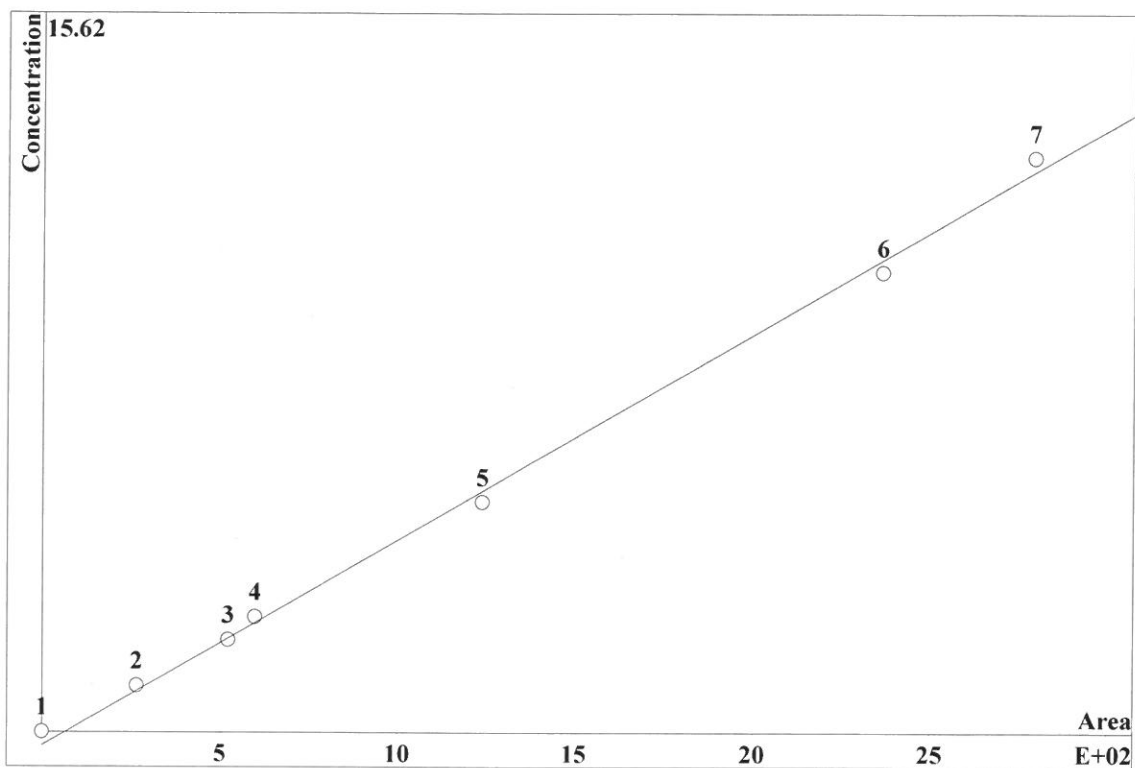

K3 = 0 K2 = 0 K1 = 0.0894674 K0 = -6.00166

Base: Area

Ref.channel: chl

ISTD:


Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used File
1	0	0	0	0	0	0
2	7.575	265.4	1	20	20.23	
3	15.5	521.8	2	20	20.23	
4	17.48	597.1	2.5	20	20.23	
5	39.73	1239	5	20	20.23	
6	78.86	2363	10	20	20.23	
7	92.96	2793	12.5	20	20.23	

CALIBRATION OF COMPONENT SO4

Method: AnionsIC2-101121.mtw
 Equation: $Q = 0.137023 \cdot A + 21.8065$
 RSD: 2.549 %
 Correlation coefficient: 0.999646

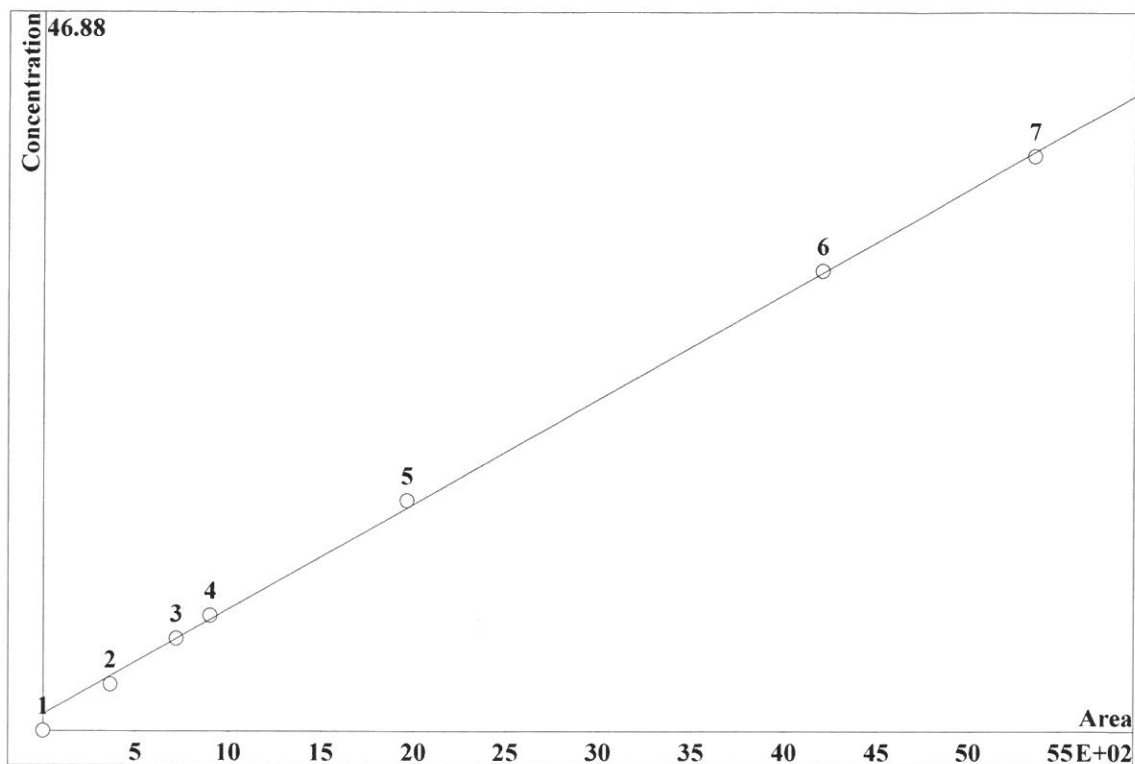

K3 = 0 K2 = 0 K1 = 0.137023 K0 = 21.8065

Base: Area

Ref.channel: chl

ISTD:

Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	12.98	361.7	3	20	23.11		
3	25.88	717.8	6	20	23.11		
4	33.03	899.9	7.5	20	23.11		
5	73.48	1959	15	20	23.11		
6	158.9	4202	30	20	23.11		
7	203.6	5354	37.5	20	23.11		

Report date: 10/13/2021 3:11:33 PM
Printed by: wet


Ident: STD1
Analysis from: 10/11/2021 8:44:43 AM
File: _2021-10-11_

Last save: 10/11/2021 12:37:14 PM

Method: AnionsIC2-101121.mtw
Run operator: wet
Analysis number: 28563

Last save: 10/11/2021 11:3

SAMPLE:
: AP/MA
Vial number: 2
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

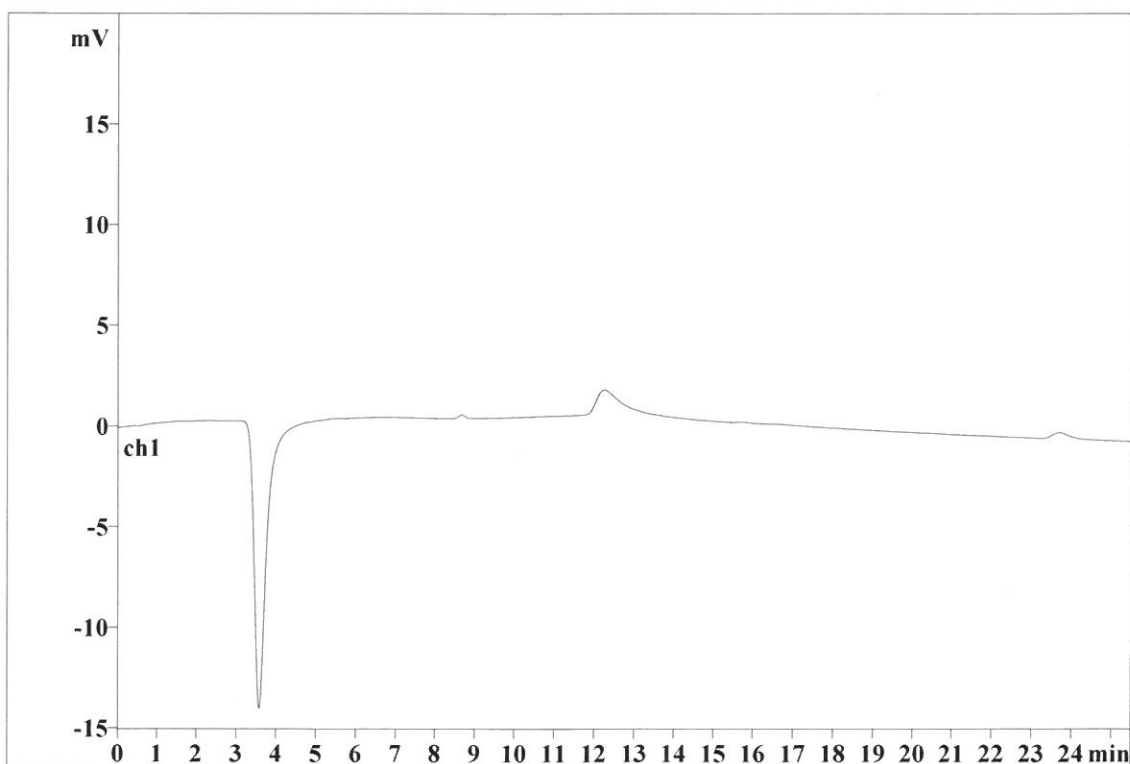

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 10/13/2021 3:11:40 PM
Printed by: wet


Ident: STD2
Analysis from: 10/11/2021 9:18:29 AM
File: _2021-10-11_

Last save: 10/11/2021 12:37:14 PM

Method: AnionsIC2-101121.mtw
Run operator: wet
Analysis number: 28564

Last save: 10/11/2021 11:3

SAMPLE:
: AP/MA
Vial number: 3
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

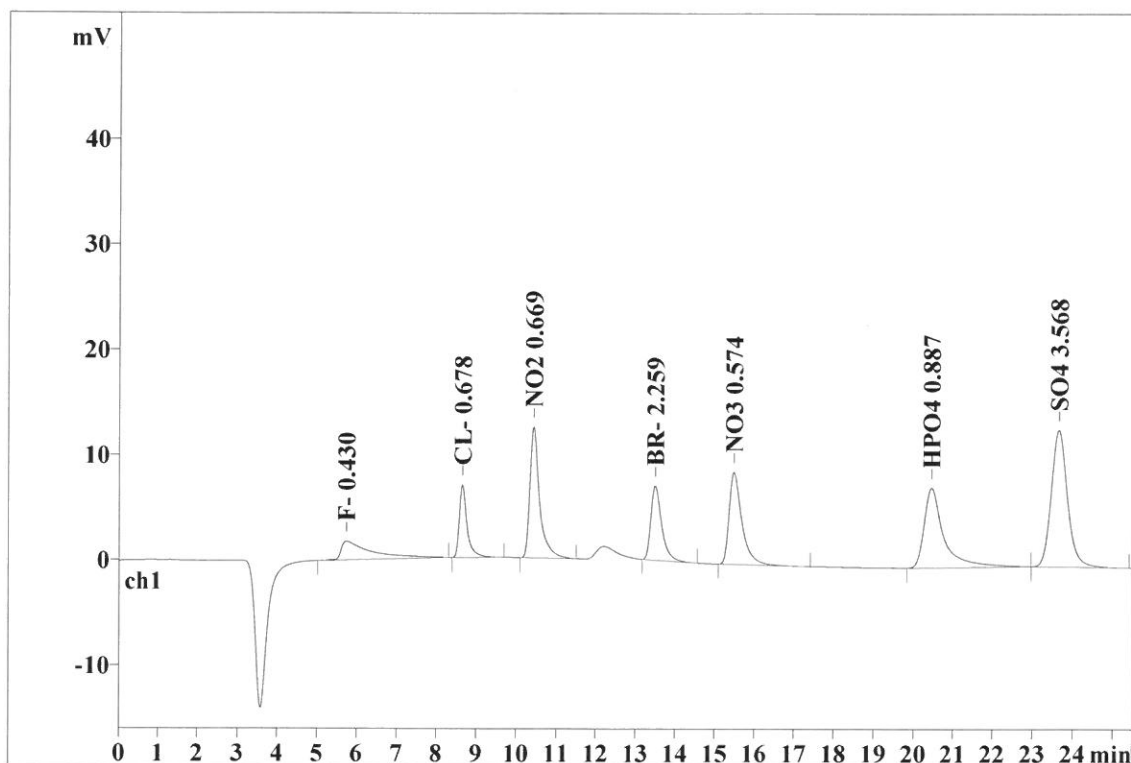

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.73	0.645	1.78	3.09	92.906	6.84
2	8.64	0.191	6.90	12.00	95.396	7.02
3	10.42	0.230	12.43	21.63	209.868	15.45
4	13.49	0.279	7.07	12.30	135.041	9.94
5	15.47	0.324	8.74	15.21	197.760	14.56
6	20.44	0.449	7.58	13.18	265.362	19.54
7	23.63	0.414	12.98	22.58	361.696	26.63
7	25.50	0.362	57.47	99.99	1358.029	100.00

This report has been created by IC Net
METROHM LTD

Report date: 10/13/2021 3:11:46 PM
Printed by: wet


Ident: STD3
Analysis from: 10/11/2021 9:46:35 AM
File: _2021-10-11_

Last save: 10/11/2021 12:37:14 PM

Method: AnionsIC2-101121.mtw
Run operator: wet
Analysis number: 28565

Last save: 10/11/2021 11:3

SAMPLE:
: AP/MA
Vial number: 4
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

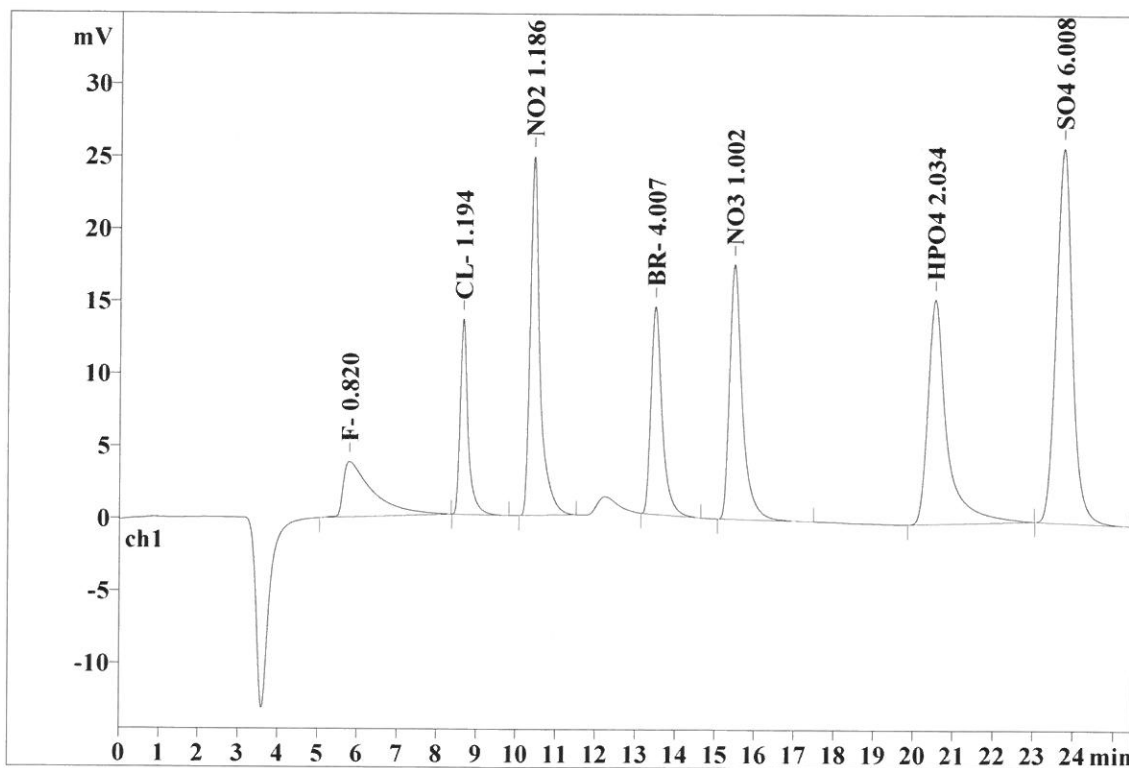

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.78	0.701	3.83	3.31	197.851	7.26
2	8.63	0.193	13.49	11.69	189.272	6.94
3	10.41	0.229	24.79	21.48	421.823	15.48
4	13.47	0.280	14.35	12.43	277.703	10.19
5	15.44	0.324	17.58	15.23	399.569	14.66
6	20.51	0.437	15.50	13.43	521.785	19.14
7	23.71	0.412	25.88	22.42	717.810	26.33
7	25.50	0.368	115.43	100.00	2725.813	100.00

This report has been created by IC Net
METROHM LTD

Report date: 10/13/2021 3:11:52 PM
Printed by: wet


Ident: STD4
Analysis from: 10/11/2021 10:14:41 AM
File: _2021-10-11_

Last save: 10/11/2021 12:37:14 PM

Method: AnionsIC2-101121.mtw
Run operator: wet
Analysis number: 28566

Last save: 10/11/2021 11:3

SAMPLE:
: AP/MA
Vial number: 5
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

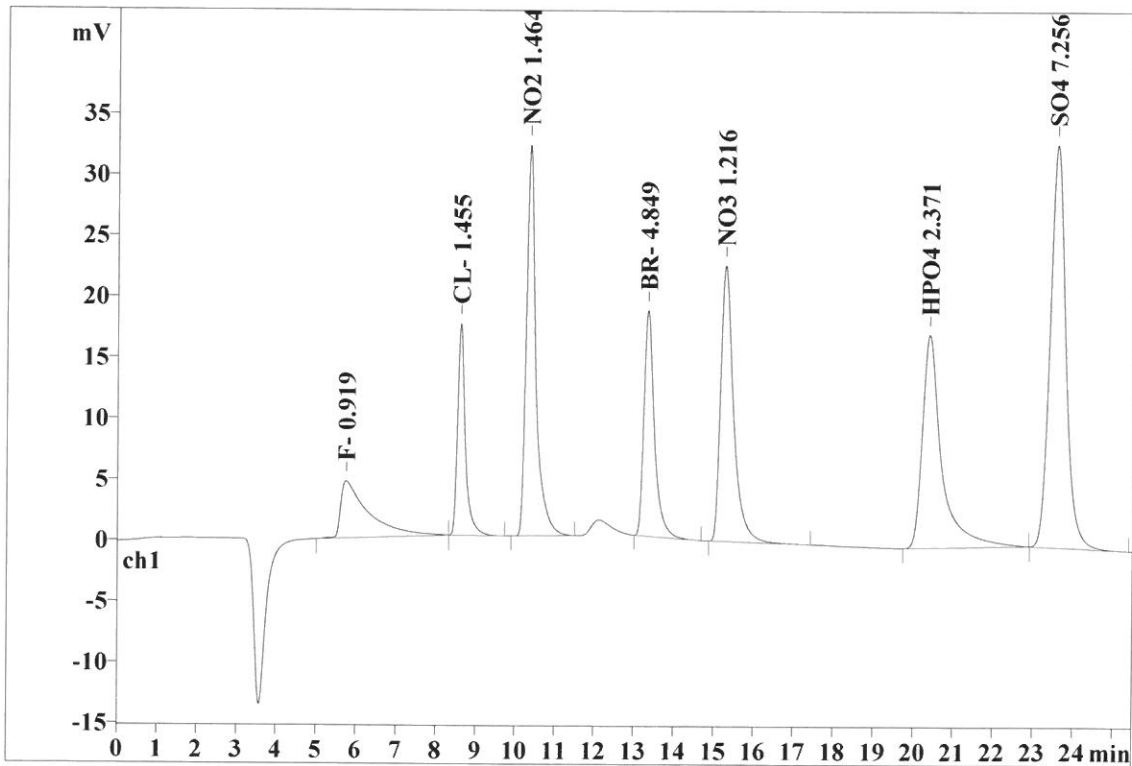

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.73	0.622	4.66	3.20	224.221	6.71
2	8.58	0.189	17.36	11.91	236.601	7.08
3	10.32	0.227	32.09	22.01	535.827	16.04
4	13.33	0.271	18.53	12.71	346.427	10.37
5	15.25	0.316	22.63	15.52	500.211	14.97
6	20.38	0.439	17.47	11.99	597.117	17.88
7	23.57	0.407	33.03	22.66	899.950	26.94
7	25.50	0.353	145.77	100.00	3340.352	100.00

This report has been created by IC Net
METROHM LTD

Report date: 10/13/2021 3:11:57 PM
Printed by: wet


Ident: STD5
Analysis from: 10/11/2021 10:42:47 AM
File: _2021-10-11_

Last save: 10/11/2021 12:37:14 PM

Method: AnionsIC2-101121.mtw
Run operator: wet
Analysis number: 28567

Last save: 10/11/2021 11:3

SAMPLE:
: AP/MA
Vial number: 6
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

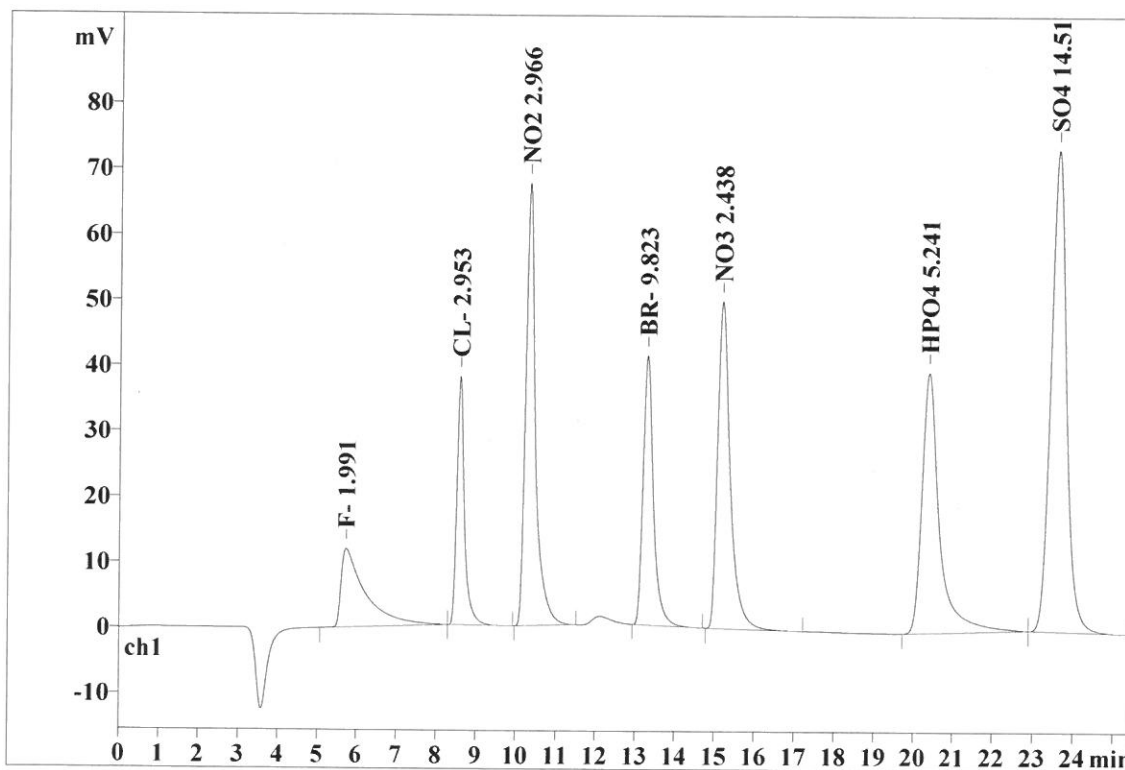

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.72	0.554	11.97	3.72	512.343	7.12
2	8.57	0.187	37.90	11.79	508.883	7.07
3	10.29	0.234	67.48	20.99	1151.409	15.99
4	13.28	0.266	41.08	12.78	752.513	10.45
5	15.16	0.309	49.87	15.51	1075.917	14.95
6	20.36	0.411	39.73	12.36	1238.702	17.21
7	23.58	0.398	73.47	22.85	1959.243	27.22
7	25.50	0.337	321.50	100.00	7199.009	100.00

This report has been created by IC Net
METROHM LTD

Report date: 10/13/2021 3:12:03 PM
Printed by: wet


Ident: STD6
Analysis from: 10/11/2021 11:10:54 AM
File: _2021-10-11_

Last save: 10/11/2021 12:37:14 PM

Method: AnionsIC2-101121.mtw
Run operator: wet
Analysis number: 28568

Last save: 10/11/2021 11:3

SAMPLE:
: AP/MA
Vial number: 7
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

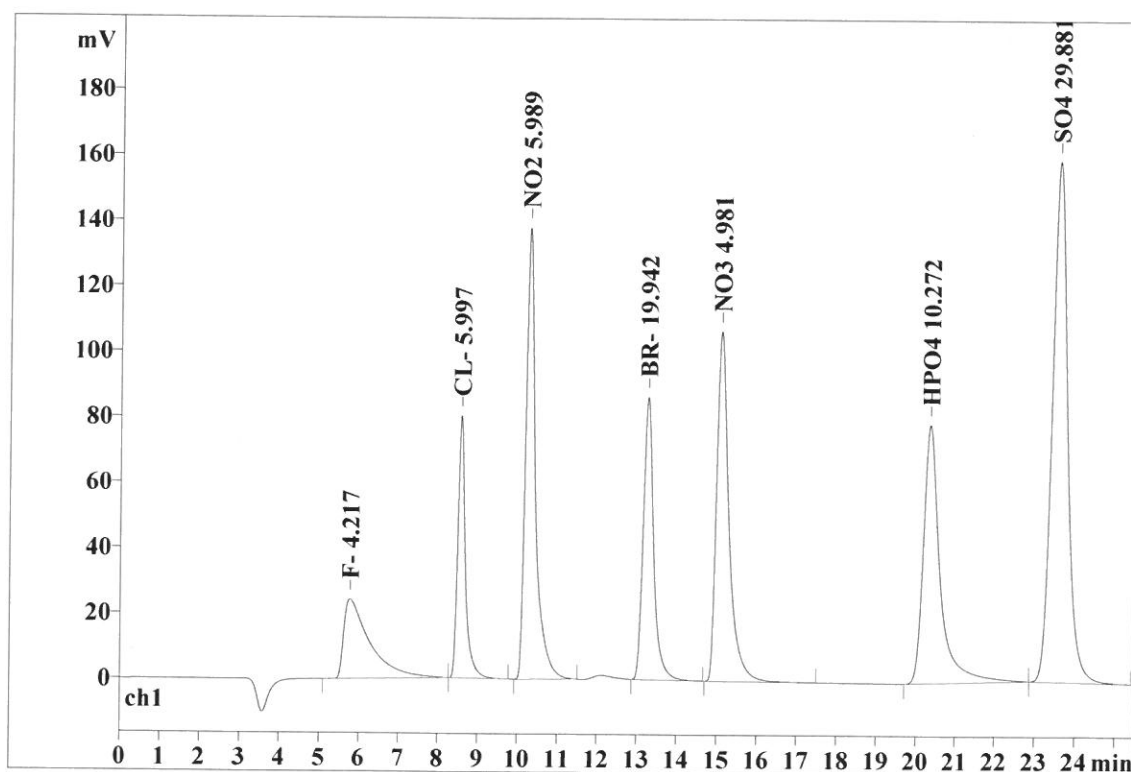

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.76	0.627	24.28	3.61	1110.305	7.41
2	8.56	0.183	80.05	11.89	1062.370	7.09
3	10.26	0.237	137.89	20.49	2390.088	15.95
4	13.24	0.266	86.24	12.81	1578.541	10.54
5	15.07	0.303	106.74	15.86	2273.277	15.18
6	20.33	0.398	78.86	11.72	2363.242	15.78
7	23.56	0.393	158.91	23.61	4202.375	28.05
7	25.50	0.344	672.96	100.00	14980.198	100.00

This report has been created by IC Net
METROHM LTD

Report date: 10/13/2021 3:12:10 PM
Printed by: wet


Ident: STD7
Analysis from: 10/11/2021 11:38:59 AM
File: _2021-10-11_

Last save: 10/11/2021 12:37:14 PM

Method: AnionsIC2-101121.mtw
Run operator: wet
Analysis number: 28569

Last save: 10/11/2021 11:3

SAMPLE:
: AP/MA
Vial number: 8
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

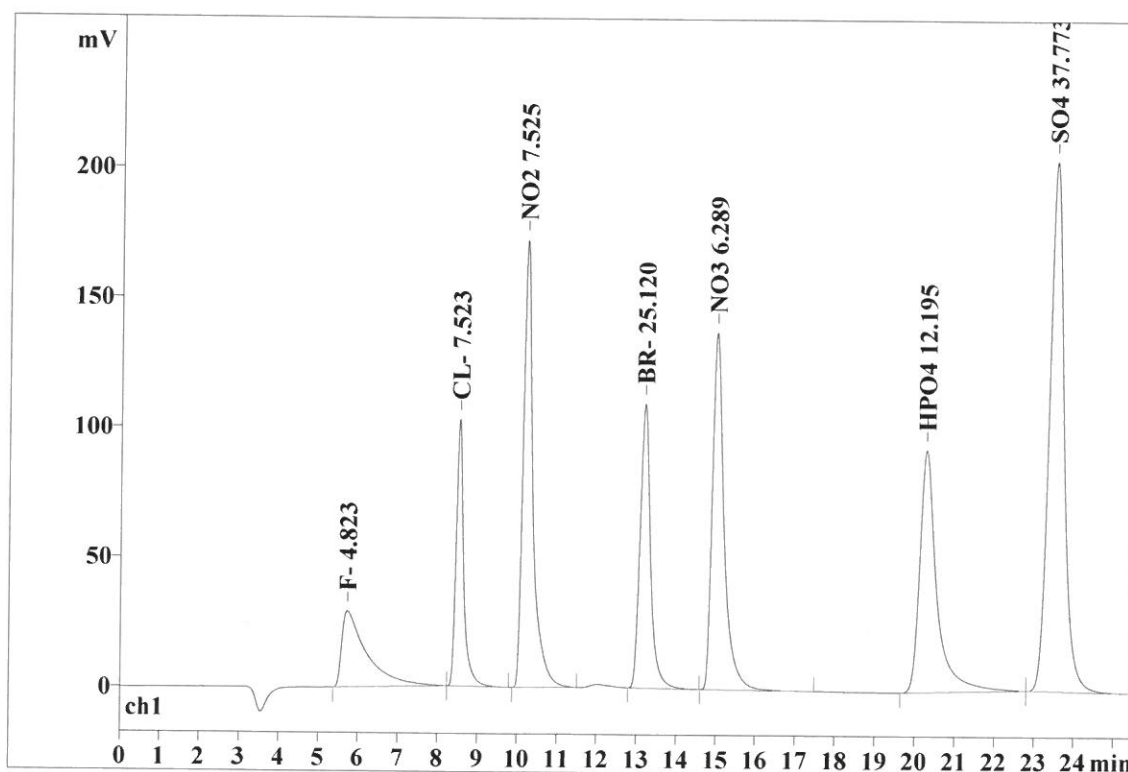

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.72	0.579	29.23	3.45	1272.991	6.82
2	8.51	0.180	102.53	12.11	1339.725	7.18
3	10.19	0.240	171.97	20.31	3019.898	16.17
4	13.17	0.266	109.19	12.90	2001.159	10.72
5	14.98	0.298	137.25	16.21	2889.232	15.47
6	20.26	0.398	92.96	10.98	2793.275	14.96
7	23.49	0.391	203.59	24.04	5354.184	28.68
7	25.50	0.336	846.71	100.00	18670.463	100.00

This report has been created by IC Net
METROHM LTD

Report date: 10/13/2021 3:12:31 PM
Printed by: wet


Ident: ICV
Analysis from: 10/11/2021 12:07:05 PM
File: _2021-10-11_

Last save: 10/11/2021 12:32:35 PM

Method: AnionsIC2-101121.mtw
Run operator: wet
Analysis number: 28570

Last save: 10/11/2021 12:0

SAMPLE:
: AP/MA
Vial number: 9
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

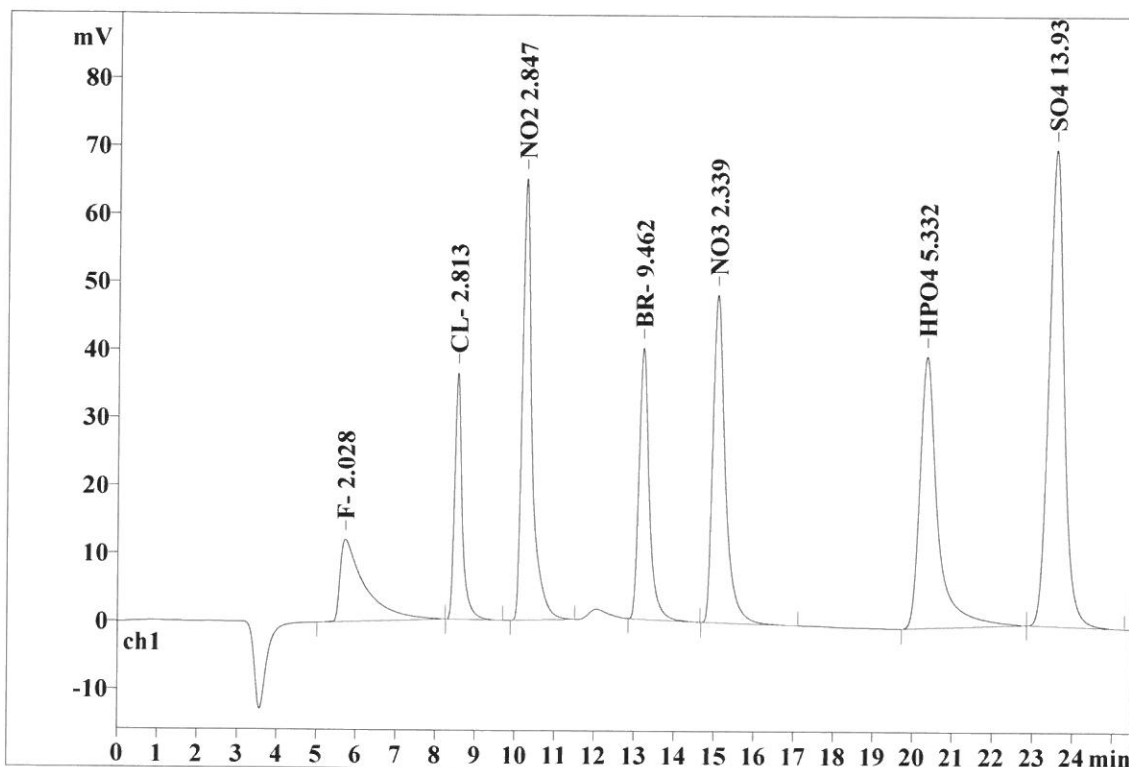

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.71	0.561	12.10	3.88	522.118	7.47
2	8.53	0.184	36.36	11.65	483.549	6.91
3	10.23	0.230	65.03	20.85	1102.404	15.76
4	13.19	0.262	39.95	12.81	723.012	10.34
5	15.04	0.304	48.29	15.48	1028.903	14.71
6	20.32	0.411	40.02	12.83	1258.914	18.00
7	23.53	0.398	70.20	22.50	1874.230	26.80
7	25.50	0.336	311.95	100.00	6993.130	100.00

This report has been created by IC Net
METROHM LTD

Report date: 10/13/2021 3:12:40 PM
Printed by: wet


Ident: ICB
Analysis from: 10/11/2021 12:35:11 PM
File: _2021-10-11_

Last save: 10/11/2021 1:00:41 PM

Method: AnionsIC2-101121.mtw
Run operator: wet
Analysis number: 28571

Last save: 10/11/2021 12:0

SAMPLE:
: AP/MA
Vial number: 10
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

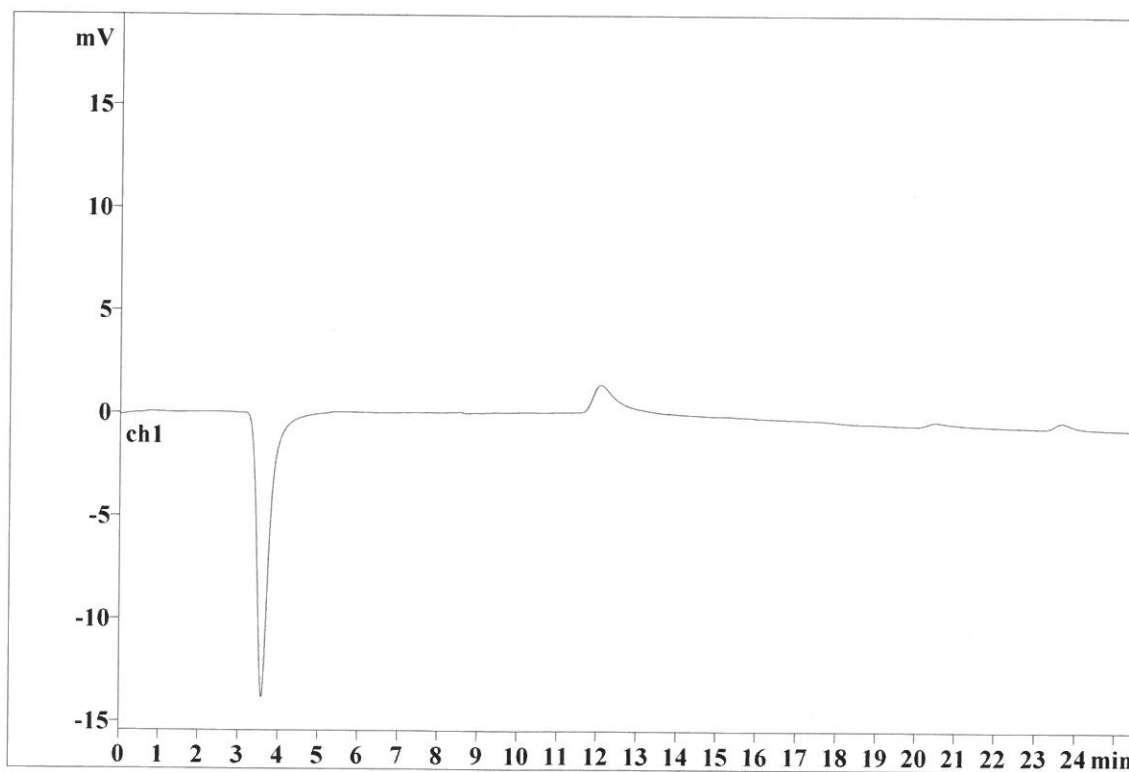

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 10/14/2021 3:34:51 PM
Printed by: wet


Ident: CCV
Analysis from: 10/14/2021 8:21:57 AM
File: _2021-10-14_

Last save: 10/14/2021 8:47:28 AM

Method: AnionsIC2-101121.mtw
Run operator: wet
Analysis number: 28603

Last save: 10/11/2021 12:3

SAMPLE:
: AP/MA
Vial number: 11
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

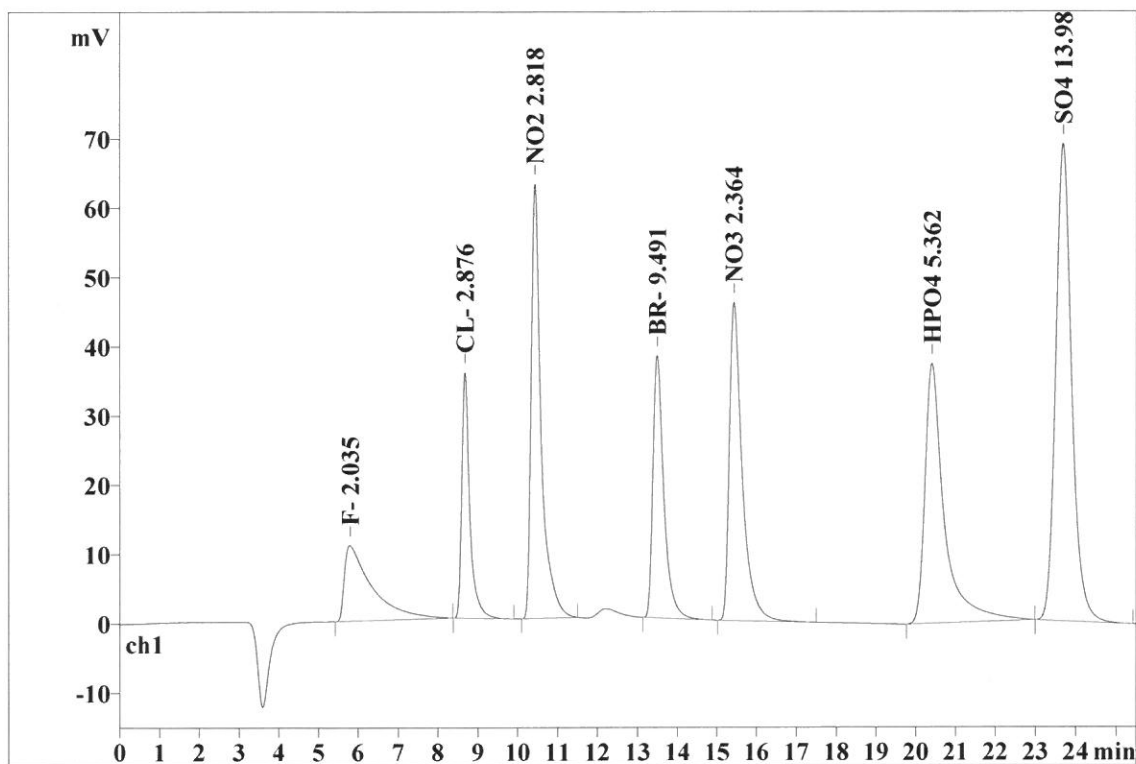

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.79	0.641	10.91	3.64	524.142	7.46
2	8.67	0.192	35.45	11.84	495.016	7.05
3	10.43	0.234	62.73	20.95	1090.513	15.53
4	13.49	0.277	37.89	12.66	725.391	10.33
5	15.42	0.323	45.95	15.35	1040.938	14.82
6	20.40	0.434	37.51	12.53	1265.744	18.02
7	23.68	0.406	68.92	23.02	1881.848	26.79
7	25.50	0.358	299.35	100.00	7023.593	100.00

This report has been created by IC Net
METROHM LTD

Report date: 10/14/2021 3:34:59 PM
Printed by: wet


Ident: CCB
Analysis from: 10/14/2021 8:50:25 AM
File: _2021-10-14_

Last save: 10/14/2021 9:15:55 AM

Method: AnionsIC2-101121.mtw
Run operator: wet
Analysis number: 28604

Last save: 10/11/2021 12:3

SAMPLE:
: AP/MA
Vial number: 12
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

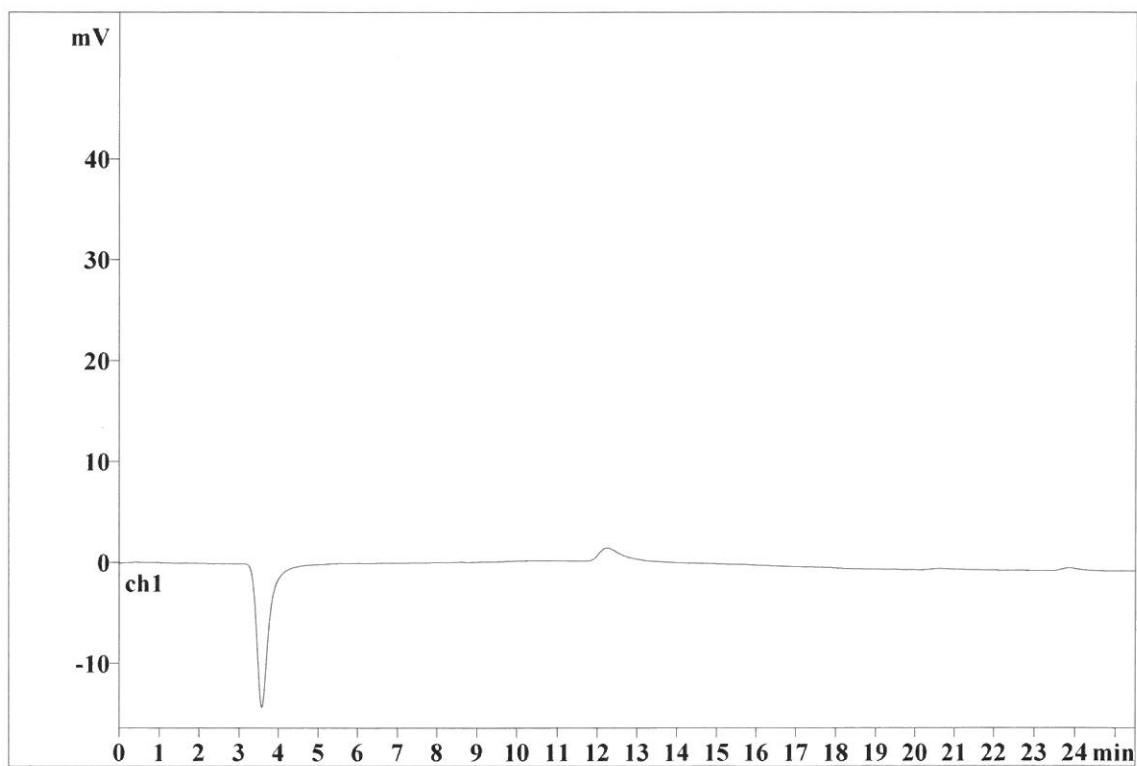

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 10/14/2021 3:35:07 PM
Printed by: wet


Ident: LB116839BLW
Analysis from: 10/14/2021 9:18:30 AM
File: _2021-10-14_

Last save: 10/14/2021 2:41:17 PM

Method: AnionsIC2-101121.mtw
Run operator: wet
Analysis number: 28605

Last save: 10/11/2021 12:3

SAMPLE:
: AP/MA
Vial number: 13
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

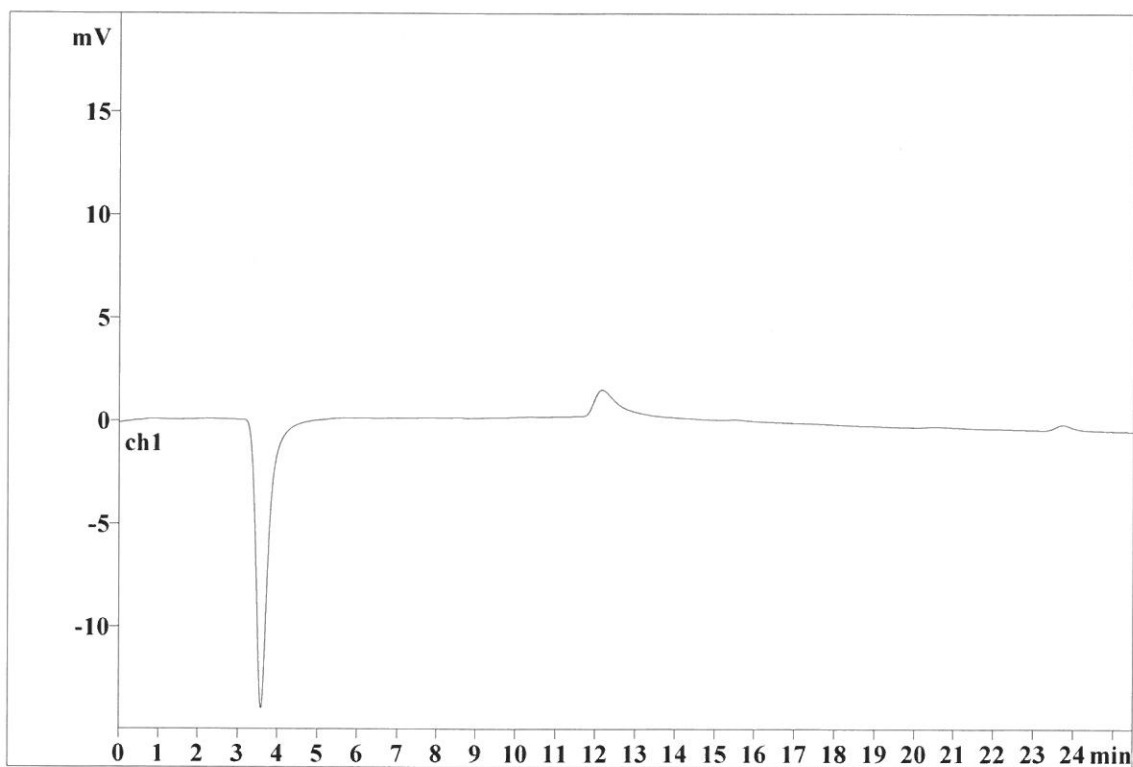

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 10/14/2021 3:35:14 PM
Printed by: wet


Ident: LB116839BSW
Analysis from: 10/14/2021 9:46:35 AM
File: _2021-10-14_

Last save: 10/14/2021 2:41:17 PM

Method: AnionsIC2-101121.mtw
Run operator: wet
Analysis number: 28606

Last save: 10/11/2021 12:3

SAMPLE:
: AP/MA
Vial number: 14
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

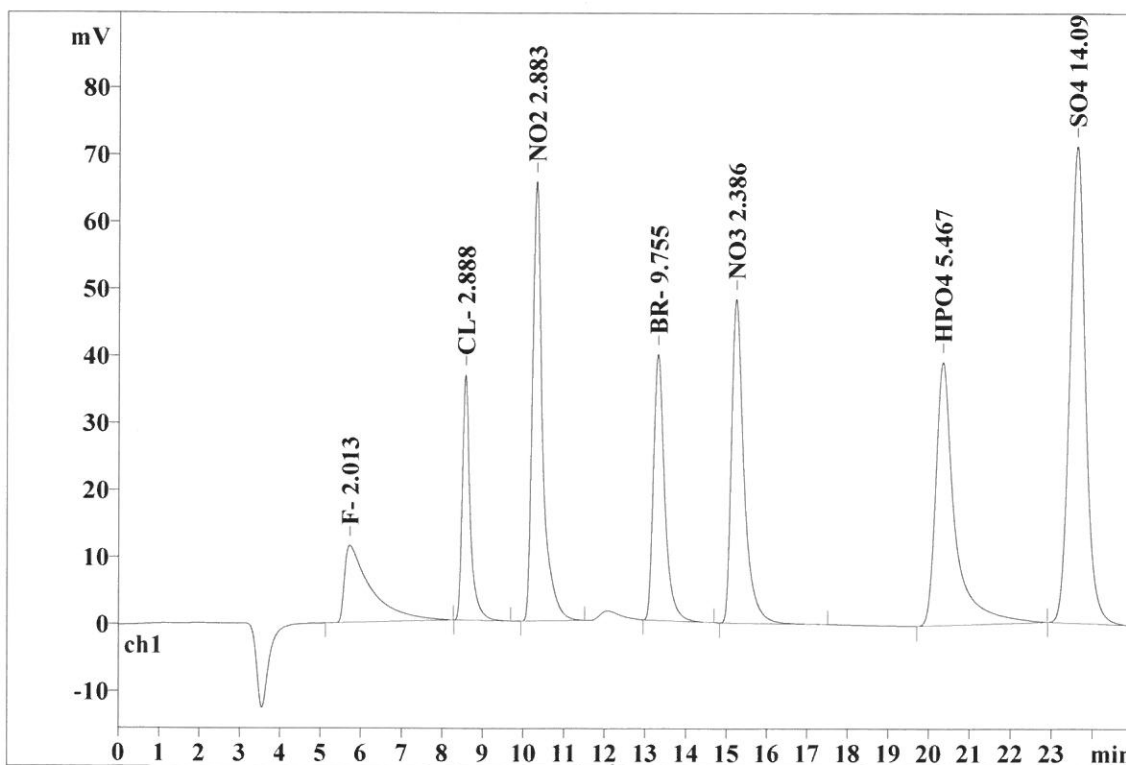

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.72	0.595	11.48	3.68	518.215	7.28
2	8.55	0.188	36.57	11.73	497.087	6.98
3	10.28	0.231	65.49	21.00	1117.418	15.70
4	13.29	0.274	39.65	12.72	746.926	10.49
5	15.21	0.312	48.27	15.48	1051.214	14.77
6	20.32	0.423	39.25	12.59	1289.188	18.11
7	23.58	0.399	71.08	22.80	1898.078	26.67
7	25.00	0.346	311.78	100.00	7118.128	100.00

This report has been created by IC Net
METROHM LTD

Report date: 10/14/2021 3:35:21 PM
Printed by: wet


Ident: M4230-01
Analysis from: 10/14/2021 1:03:57 PM
File: _2021-10-14_

Last save: 10/14/2021 1:29:28 PM

Method: AnionsIC2-101121.mtw
Run operator: wet
Analysis number: 28608

Last save: 10/11/2021 12:3

SAMPLE:
: AP/MA
Vial number: 15
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

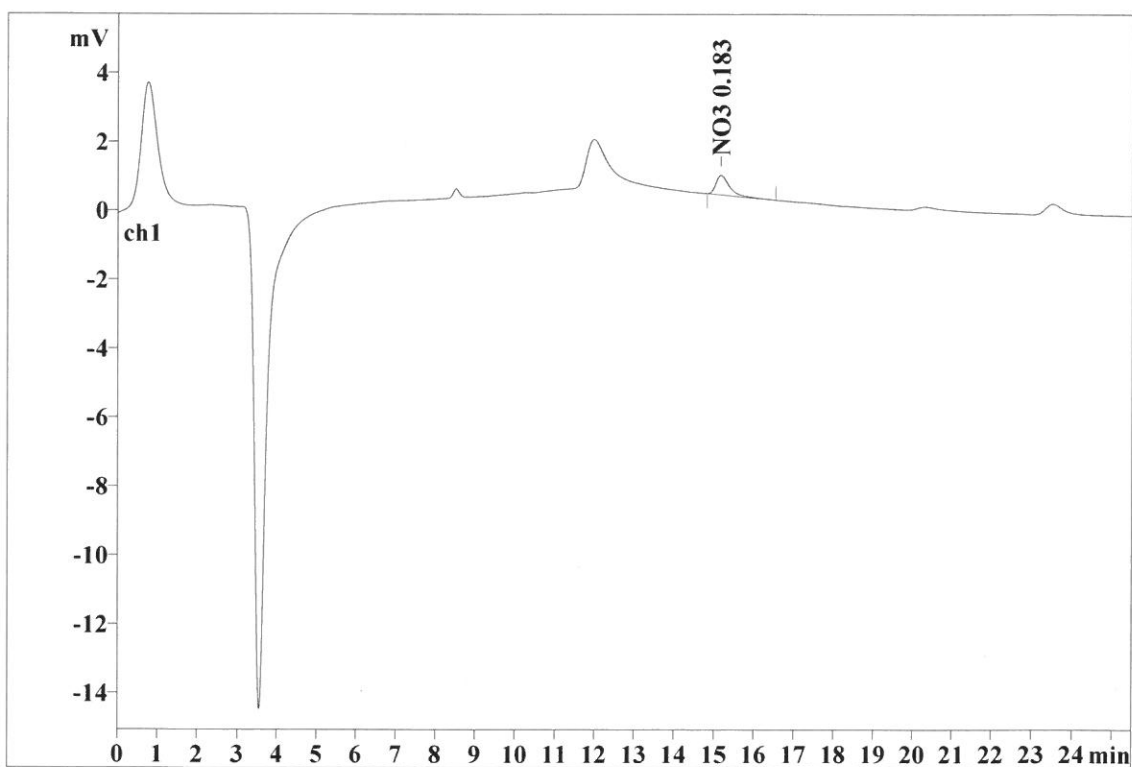

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	0.00	0.000	0.00	0.00	0.000	0.00
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	15.14	0.331	0.57	99.93	13.451	100.00
6	0.00	0.000	0.00	0.00	0.000	0.00
7	0.00	0.000	0.00	0.00	0.000	0.00
7	25.50	0.047	0.57	99.93	13.451	100.00

This report has been created by IC Net
METROHM LTD

Report date: 10/14/2021 3:35:28 PM
Printed by: wet


Ident: M4230-01MS
Analysis from: 10/14/2021 1:38:22 PM
File: _2021-10-14_

Last save: 10/14/2021 2:03:52 PM

Method: AnionsIC2-101121.mtw
Run operator: wet
Analysis number: 28609

Last save: 10/11/2021 12:3

SAMPLE:
: AP/MA
Vial number: 16
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

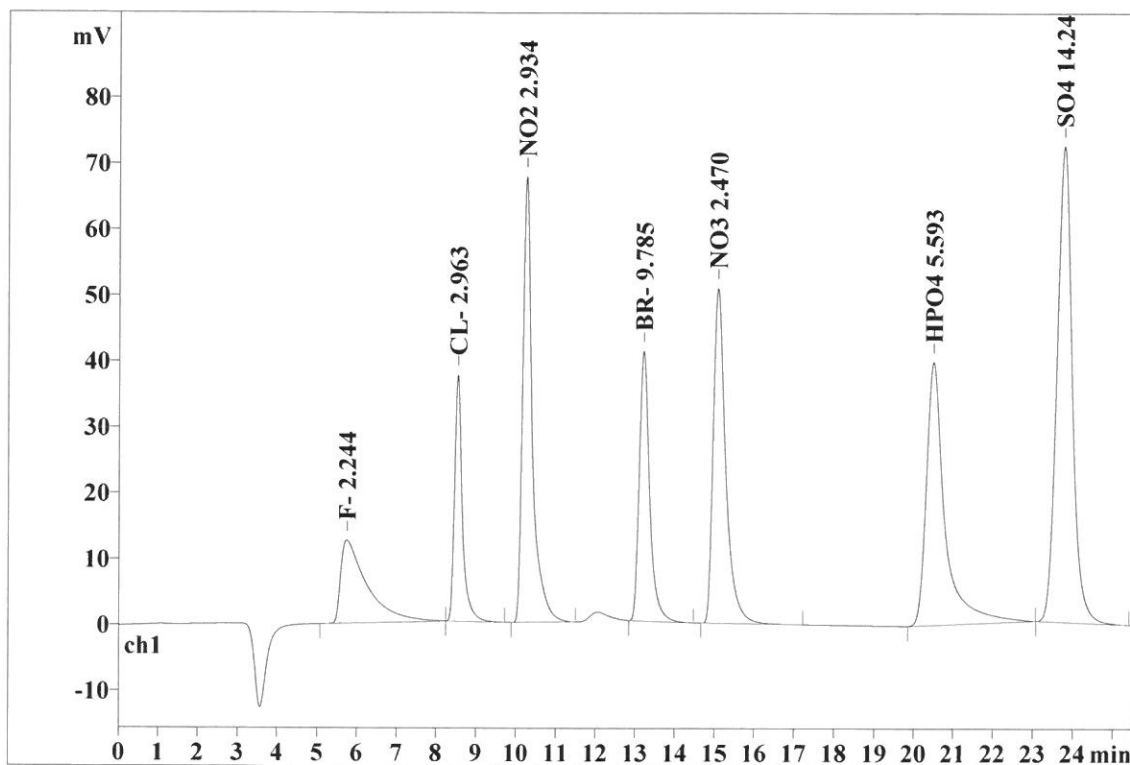

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.74	0.630	12.58	3.92	580.246	7.94
2	8.52	0.189	37.35	11.62	510.713	6.99
3	10.23	0.228	67.59	21.03	1137.984	15.57
4	13.20	0.266	40.94	12.74	749.367	10.26
5	15.06	0.308	50.84	15.82	1090.837	14.93
6	20.47	0.424	39.90	12.41	1317.269	18.03
7	23.74	0.396	72.20	22.46	1920.442	26.28
7	25.50	0.349	321.39	100.00	7306.858	100.00

This report has been created by IC Net
METROHM LTD

Report date: 10/14/2021 3:35:34 PM
Printed by: wet


Ident: M4230-01MSD
Analysis from: 10/14/2021 2:06:27 PM
File: _2021-10-14_

Last save: 10/14/2021 2:31:57 PM

Method: AnionsIC2-101121.mtw
Run operator: wet
Analysis number: 28610

Last save: 10/11/2021 12:3

SAMPLE:
: AP/MA
Vial number: 17
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

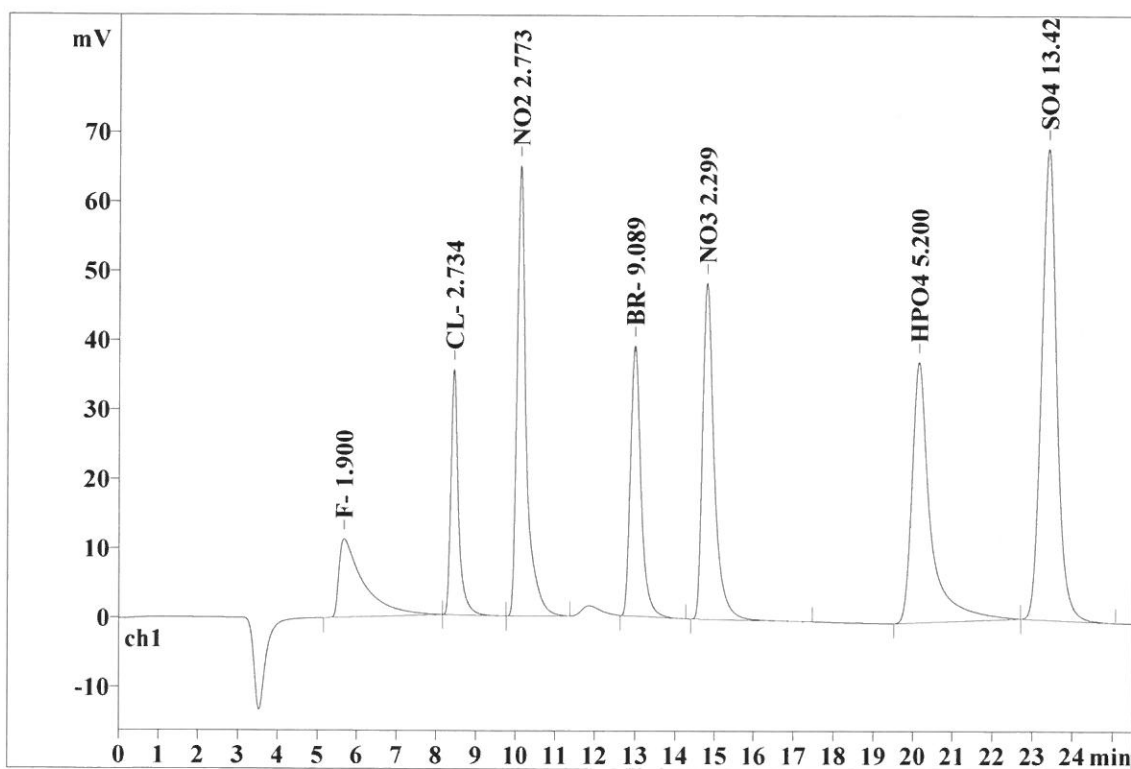

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.66	0.568	11.30	3.71	487.918	7.22
2	8.42	0.183	35.43	11.63	469.121	6.94
3	10.09	0.223	64.90	21.31	1072.359	15.86
4	12.97	0.259	38.95	12.79	692.531	10.24
5	14.77	0.298	48.46	15.91	1010.088	14.94
6	20.12	0.417	37.55	12.33	1229.487	18.18
7	23.37	0.395	67.94	22.31	1800.598	26.63
7	25.50	0.335	304.53	100.00	6762.102	100.00

This report has been created by IC Net
METROHM LTD

Report date: 10/14/2021 3:35:41 PM
Printed by: wet


Ident: CCV
Analysis from: 10/14/2021 2:35:21 PM
File: _2021-10-14_

Last save: 10/14/2021 3:00:52 PM

Method: AnionsIC2-101121.mtw
Run operator: wet
Analysis number: 28611

Last save: 10/11/2021 12:3

SAMPLE:
: AP/MA
Vial number: 11
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

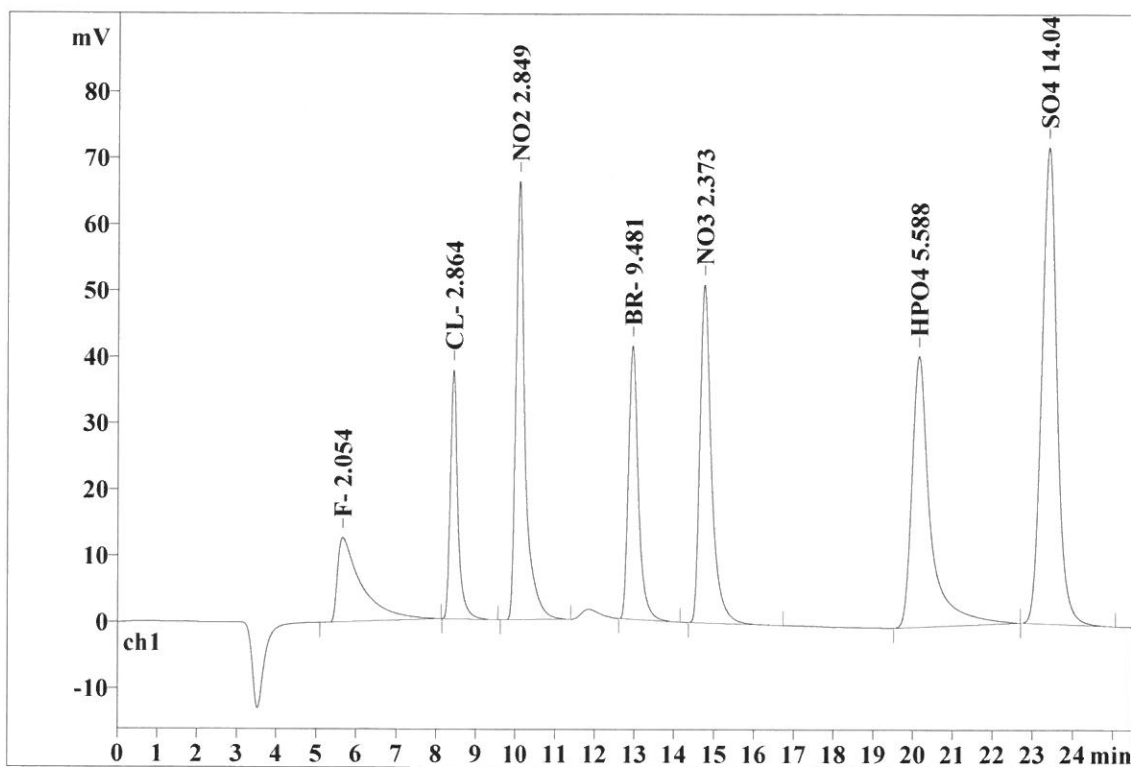

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.65	0.544	12.71	3.95	529.295	7.45
2	8.41	0.182	37.61	11.69	492.847	6.94
3	10.07	0.227	66.17	20.57	1103.448	15.54
4	12.93	0.257	41.31	12.84	724.592	10.20
5	14.72	0.295	51.05	15.87	1044.919	14.71
6	20.12	0.413	40.90	12.71	1316.243	18.53
7	23.37	0.392	71.94	22.36	1890.134	26.62
7	25.50	0.330	321.69	100.00	7101.479	100.00

This report has been created by IC Net
METROHM LTD

Report date: 10/14/2021 3:35:50 PM
Printed by: wet


Ident: CCB
Analysis from: 10/14/2021 3:03:27 PM
File: _2021-10-14_

Last save: 10/14/2021 3:28:57 PM

Method: AnionsIC2-101121.mtw
Run operator: wet
Analysis number: 28612

Last save: 10/11/2021 12:3

SAMPLE:
: AP/MA
Vial number: 12
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

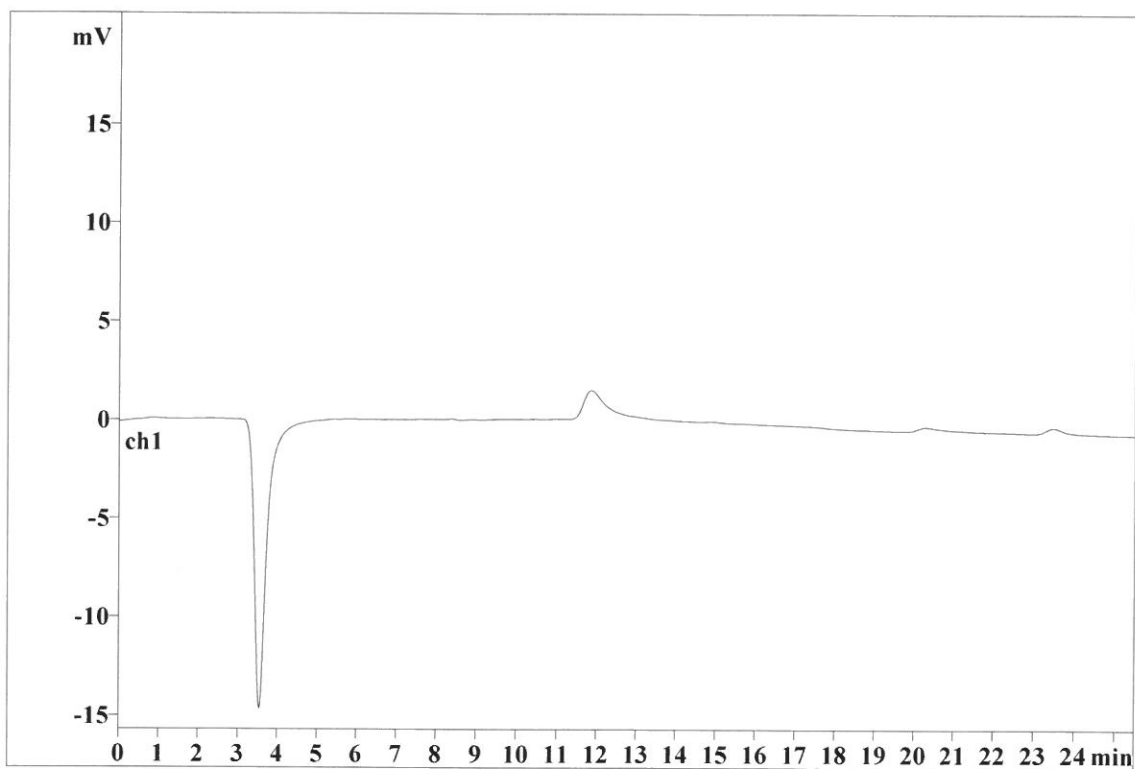

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD