


LB116920

7471B

INSTRUMENT ID: CV1

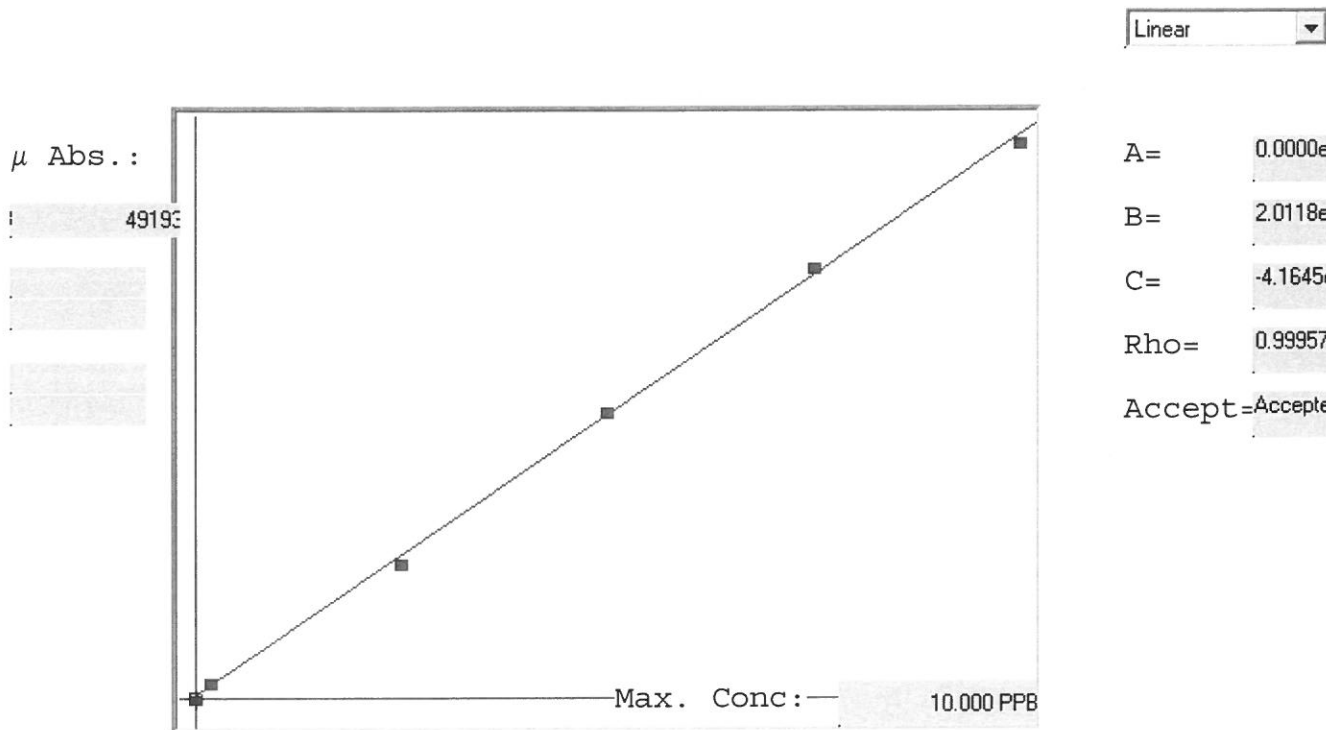

A= 0.0000e+000

B= 2.0118e-004

C= -4.1645e-002

Rho= 0.9995738

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	-0.033	-0.033	41	0.000	41					19
0.2	0.200	0.238	0.038	1390	0.0 %	1390					-4
2.5	2.500	2.389	-0.111	12081	0.0 %	12081					2
5.0	5.000	5.094	0.094	25530	0.0 %	25530					2
7.5	7.500	7.657	0.157	38269	0.0 %	38269					-1
10.0	10.000	9.855	-0.145	49193	0.0 %	49193					

LB116920 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 20 Oct 2021 09:01:26

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	41	-	0.0000	7471B	PPB	20 Oct 2021 09:06:22	S	Std
0.2 - 1	51.2	1390	-	0.2000	7471B	PPB	20 Oct 2021 09:08:39	S	Std
2.5 - 1	52.5	12081	-	2.5000	7471B	PPB	20 Oct 2021 09:10:56	S	Std
5.0 - 1	55	25530	-	5.0000	7471B	PPB	20 Oct 2021 09:13:13	S	Std
7.5 - 1	57.5	38269	-	7.5000	7471B	PPB	20 Oct 2021 09:15:29	S	Std
10.0 - 1	511	49193	-	10.0000	7471B	PPB	20 Oct 2021 09:17:46	S	Std
ICV50 - 1	ICV50	20939	4.1708	-7471B	PPB	PPB	20 Oct 2021 09:20:25	U	SMPL
ICB50 - 1	ICB50	-279	-0.0978	-7471B	PPB	PPB	20 Oct 2021 09:22:40	U	SMPL
CCV99 - 1	CCV99	25547	5.0979	-7471B	PPB	PPB	20 Oct 2021 09:24:54	U	SMPL
CCB99 - 1	CCB99	-122	-0.0662	-7471B	PPB	PPB	20 Oct 2021 09:27:09	U	SMPL
CRA - 1	CRA	1352	0.2303	-7471B	PPB	PPB	20 Oct 2021 09:29:24	U	SMPL
HighStd - 1	HighStd	49136	9.8435	-7471B	PPB	PPB	20 Oct 2021 09:31:39	U	SMPL
ChkStd - 1	ChkStd	35921	7.1849	-7471B	PPB	PPB	20 Oct 2021 09:33:54	U	SMPL
PB140063BL - 1	PBS	271	0.0129	-7471B	PPB	PPB	20 Oct 2021 09:36:11	U	SMPL
PB140063BS - 1	LCSS	21366	4.2567	-7471B	PPB	PPB	20 Oct 2021 09:38:28	U	SMPL
M4269-01 - 1	RT-4197	5999	1.1652	-7471B	PPB	PPB	20 Oct 2021 09:40:45	U	SMPL
M4269-01DUP - 1	RT-4197DUP	5495	1.0638	-7471B	PPB	PPB	20 Oct 2021 09:43:00	U	SMPL
M4269-01MS - 1	RT-4197MS	26548	5.2992	-7471B	PPB	PPB	20 Oct 2021 09:45:17	U	SMPL
M4269-01MSD - 1	RT-4197MSD	26241	5.2375	-7471B	PPB	PPB	20 Oct 2021 09:47:34	U	SMPL
M4271-01 - 1	OK-01-101821	1886	0.3378	-7471B	PPB	PPB	20 Oct 2021 09:49:50	U	SMPL
CCV100 - 1 CCV01	CCV100 CCV01	25315	5.0512	-7471B	PPB	PPB	20 Oct 2021 09:52:05	U	SMPL
CCB100 - 1 CCB01	CCB100 CCB01	-47	-0.0511	-7471B	PPB	PPB	20 Oct 2021 09:54:20	U	SMPL
M4273-01 - 1	R-LA-4/2-WC	6029	1.1713	-7471B	PPB	PPB	20 Oct 2021 09:56:36	U	SMPL
M4274-01 - 1	WC-2-BS	35930	7.1867	-7471B	PPB	PPB	20 Oct 2021 09:58:51	U	SMPL
M4274-04 - 1	WC-2-CS	7666	1.5006	-7471B	PPB	PPB	20 Oct 2021 10:01:07	U	SMPL
M4274-07 - 1	WC-2-DS	25008	4.9894	-7471B	PPB	PPB	20 Oct 2021 10:03:22	U	SMPL
M4269-01LX5 - 1		967	0.1529	-7471B	PPB	PPB	20 Oct 2021 10:05:38	U	SMPL
M4269-01A - 1		26434	5.2763	-7471B	PPB	PPB	20 Oct 2021 10:07:55	U	SMPL
CCV101 - 1 CCB02	CCV101 CCB02	25547	5.0979	-7471B	PPB	PPB	20 Oct 2021 10:10:11	U	SMPL
CCB101 - 1 CCB02	CCB101 CCB02	-50	-0.0517	-7471B	PPB	PPB	20 Oct 2021 10:12:28	U	SMPL

MS
16/10/21