

=====

LB116928

Page: 1

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092Reviewed by : nb Instrument ID : Konelab10/20/2021 15:21
=====

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	96.378	0.0	0.070	
ICB1	-0.779	0.0	0.001	
CCV1	236.475	0.0	0.169	
CCB1	-0.698	0.0	0.001	
PB140076BL	-0.605	0.0	0.001	
PB140076BS	99.996	0.0	0.072	
M4274-01	-0.415	0.0	0.001	
M4274-01DUP	-0.779	0.0	0.001	
M4274-01MS	39.428	0.0	0.029	
M4274-01MSD	40.225	0.0	0.030	
M4274-04	0.030	0.0	0.001	
M4274-07	0.623	0.0	0.002	
CCV2	238.594	0.0	0.170	
CCB2	-0.745	0.0	0.001	
M4285-01	-0.512	0.0	0.001	
M4285-04	-0.819	0.0	0.001	
M4285-07	-0.641	0.0	0.001	
M4285-13	-0.854	0.0	0.001	
M4285-16	-0.867	0.0	0.001	
LOWPB140076	9.349	0.0	0.008	
HIGHPB140076	512.919	0.0	0.365	
M4285-10	-0.154	0.0	0.001	
CCV3	262.195	0.0	0.187	
CCB3	-0.984	0.0	0.001	

93% (20-1107) OK
103%
Test limit high

N	24
Mean	63.640
SD	126.8400
CV%	199.31

Aquakem v. 7.2AQ1

Results from time period:

Wed Oct 20 13:05:42 2021

Wed Oct 20 15:20:49 2021

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Total CN	P	-0.4934	µg/l	10/20/2021 14:15:35	
5.OPPBCN	A	Total CN	P	4.3485	µg/l	10/20/2021 14:15:36	
10PPBCN	A	Total CN	P	9.0944	µg/l	10/20/2021 14:15:37	
50PPBCN	A	Total CN	P	48.639	µg/l	10/20/2021 14:15:38	
100PPBCN	A	Total CN	P	103.4707	µg/l	10/20/2021 14:15:39	
250PPBCN	A	Total CN	P	250.9485	µg/l	10/20/2021 14:15:40	
500PPBCN	A	Total CN	P	498.9923	µg/l	10/20/2021 14:15:41	
ICV1	S	Total CN	P	96.3779	µg/l	10/20/2021 14:46:39	
ICB1	S	Total CN	P	-0.7794	µg/l	10/20/2021 14:46:41	
CCV1	S	Total CN	P	236.4747	µg/l	10/20/2021 14:46:43	
CCB1	S	Total CN	P	-0.6975	µg/l	10/20/2021 14:46:44	
PB140076BL	S	Total CN	P	-0.6051	µg/l	10/20/2021 14:46:46	
PB140076BS	S	Total CN	P	99.9956	µg/l	10/20/2021 14:46:48	
M4274-01	S	Total CN	P	-0.4154	µg/l	10/20/2021 14:54:15	
M4274-01DUP	S	Total CN	P	-0.7794	µg/l	10/20/2021 14:54:16	
M4274-01MS	S	Total CN	P	39.4282	µg/l	10/20/2021 14:54:17	
M4274-01MSD	S	Total CN	P	40.2246	µg/l	10/20/2021 14:54:18	
M4274-04	S	Total CN	P	0.0305	µg/l	10/20/2021 14:54:21	
M4274-07	S	Total CN	P	0.6227	µg/l	10/20/2021 14:54:22	
CCV2	S	Total CN	P	238.5937	µg/l	10/20/2021 14:54:23	
CCB2	S	Total CN	P	-0.7451	µg/l	10/20/2021 14:59:00	
M4285-01	S	Total CN	P	-0.5121	µg/l	10/20/2021 14:59:01	
M4285-04	S	Total CN	P	-0.8192	µg/l	10/20/2021 14:59:02	
M4285-07	S	Total CN	P	-0.6412	µg/l	10/20/2021 14:59:03	
M4285-13	S	Total CN	P	-0.854	µg/l	10/20/2021 15:05:04	
M4285-16	S	Total CN	P	-0.8673	µg/l	10/20/2021 15:05:05	
LOWPB140076	S	Total CN	P	9.3486	µg/l	10/20/2021 15:10:13	
HIGHPB140076	S	Total CN	P	512.9185	µg/l	10/20/2021 15:10:14	
M4285-10	S	Total CN	P	-0.154	µg/l	10/20/2021 15:13:00	
CCV3	S	Total CN	P	262.1952	µg/l	10/20/2021 15:18:50	
CCB3	S	Total CN	P	-0.9842	µg/l	10/20/2021 15:20:49	

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : *AS*

Instrument ID : Konelab

10/20/2021 14:16


Test Total CN

Accepted 10/20/2021 14:16

Factor 1410
Bias 0.001

Coeff. of det. 0.999916

Errors

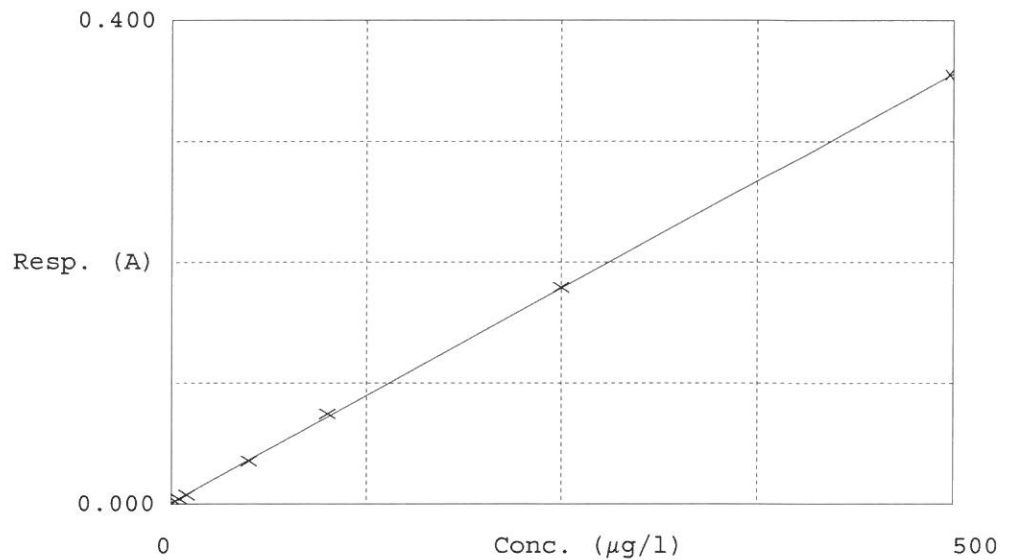

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.001	-0.4934	0.0000	
2	5.0PPBCN	0.004	4.3485	5.0000	
3	10PPBCN	0.008	9.0944	10.0000	
4	50PPBCN	0.036	48.6390	50.0000	
5	100PPBCN	0.075	103.4707	100.0000	
6	250PPBCN	0.179	250.9485	250.0000	
7	500PPBCN	0.355	498.9923	500.0000	

del
Errors

-13.0
-9.1
-2.8
3.5
0.4
-0.2

AS
10/20/21