


LB 116941

7471B

INSTRUMENT ID: CV2

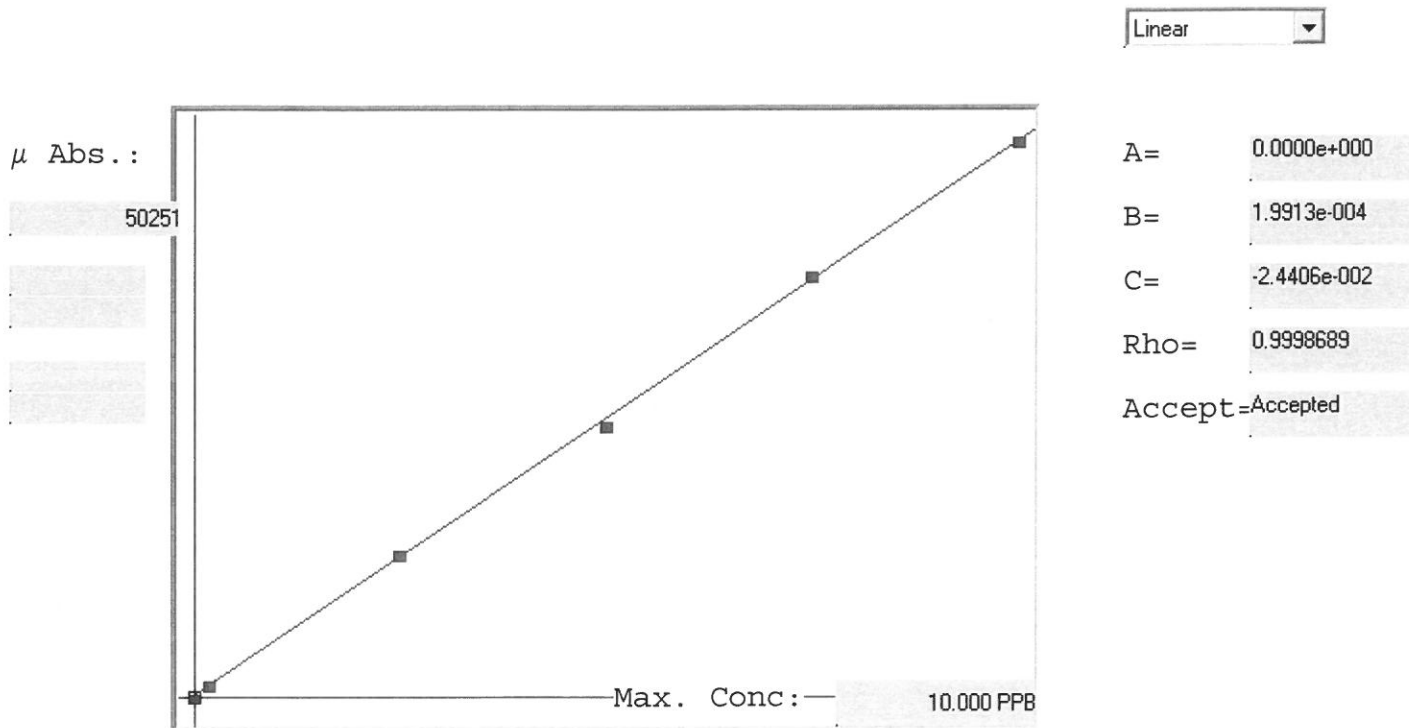

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	o/b
0.0	0.000	0.005	0.005	146	0.000	146					-
0.2	0.200	0.203	0.003	1143	0.0 %	1143					2
2.5	2.500	2.540	0.040	12877	0.0 %	12877					2
5.0	5.000	4.888	-0.112	24668	0.0 %	24668					-2
7.5	7.500	7.583	0.083	38203	0.0 %	38203					1
10.0	10.000	9.982	-0.018	50251	0.0 %	50251					0

LB116941 INSTRUMENT ID : CV1

Method: 7471B		Operator: Admin		Date of Analysis: 21 Oct 2021 13:25:43					
Sample ID	Extended ID	μ Abs.	Conc.	Std. Conc	Method	Units	Date	Type	Type
0.0 - 1		146	-	0.0000	7471B	PPB	21 Oct 2021 13:26:52	S	Std
0.2 - 1		1143	-	0.2000	7471B	PPB	21 Oct 2021 13:29:09	S	Std
2.5 - 1		12877	-	2.5000	7471B	PPB	21 Oct 2021 13:31:26	S	Std
5.0 - 1		24668	-	5.0000	7471B	PPB	21 Oct 2021 13:33:43	S	Std
7.5 - 1		38203	-	7.5000	7471B	PPB	21 Oct 2021 13:35:59	S	Std
10.0 - 1		50251	-	10.0000	7471B	PPB	21 Oct 2021 13:38:15	S	Std
ICV53 - 1	ICV53	20254	4.0087	-	7471B	PPB	21 Oct 2021 13:41:28	U	SMPL
ICB53 - 1	ICB53	66	-0.0113	-	7471B	PPB	21 Oct 2021 13:43:43	U	SMPL
CCV12 - 1	CCV12	24404	4.8351	-	7471B	PPB	21 Oct 2021 13:45:58	U	SMPL
CCB12 - 1	CCB12	63	-0.0119	-	7471B	PPB	21 Oct 2021 13:48:13	U	SMPL
CRA - 1	CRA	1149	0.2044	-	7471B	PPB	21 Oct 2021 13:50:28	U	SMPL
HighStd - 1	HighStd	50334	9.9984	-	7471B	PPB	21 Oct 2021 13:52:43	U	SMPL
ChkStd - 1	ChkStd	35461	7.0368	-	7471B	PPB	21 Oct 2021 13:54:58	U	SMPL
PB140094BL - 1	PBS	34	-0.0176	-	7471B	PPB	21 Oct 2021 14:01:15	U	SMPL
PB140094BS - 1	LCSS	18539	3.6672	-	7471B	PPB	21 Oct 2021 14:03:32	U	SMPL
M4280-07 - 1	2081	2757	0.5246	-	7471B	PPB	21 Oct 2021 14:05:48	U	SMPL
M4280-07DUP - 1	2081DUP	2500	0.4734	-	7471B	PPB	21 Oct 2021 14:08:06	U	SMPL
M4280-07MS - 1	2081MS	22207	4.3976	-	7471B	PPB	21 Oct 2021 14:10:23	U	SMPL
M4280-07MSD - 1	2081MSD	23756	4.7060	-	7471B	PPB	21 Oct 2021 14:12:39	U	SMPL
M4283-01 - 1	VNJ-231	216562	43.0989	-	7471B	PPB	21 Oct 2021 14:14:55	U	SMPL
CCV13 - 1	CCV13	24237	4.8018	-	7471B	PPB	21 Oct 2021 14:28:59	U	SMPL
CCB13 - 1	CCB13	60	-0.0125	-	7471B	PPB	21 Oct 2021 14:31:15	U	SMPL
M4283-04 - 1	CONCRETE-PAD	955	0.1658	-	7471B	PPB	21 Oct 2021 14:33:30	U	SMPL
M4284-01 - 1	30851-OIL	996	0.1739	-	7471B	PPB	21 Oct 2021 14:35:45	U	SMPL
M4284-02 - 1	20878-SOLID	796	0.1341	-	7471B	PPB	21 Oct 2021 14:38:00	U	SMPL
M4284-03 - 1	30852	963	0.1674	-	7471B	PPB	21 Oct 2021 14:40:16	U	SMPL
M4284-04 - 1	16943	1363	0.2470	-	7471B	PPB	21 Oct 2021 14:42:32	U	SMPL
M4285-01 - 1	MH-EA-(1)	1698	0.3137	-	7471B	PPB	21 Oct 2021 14:44:48	U	SMPL
M4285-04 - 1	MH-EB-(1)	878	0.1504	-	7471B	PPB	21 Oct 2021 14:47:04	U	SMPL
M4285-07 - 1	MH-FA-(1)	988	0.1723	-	7471B	PPB	21 Oct 2021 14:49:21	U	SMPL
M4285-10 - 1	MH-GA-(1)	5477	1.0662	-	7471B	PPB	21 Oct 2021 14:51:38	U	SMPL
M4285-13 - 1	MH-GB-(1)	4017	0.7755	-	7471B	PPB	21 Oct 2021 14:53:54	U	SMPL
CCV14 - 1	CCV14	23653	4.6855	-	7471B	PPB	21 Oct 2021 14:56:10	U	SMPL
CCB14 - 1	CCB14	104	-0.0037	-	7471B	PPB	21 Oct 2021 14:58:25	U	SMPL
M4285-16 - 1	MH-FB-(1)	1646	0.3034	-	7471B	PPB	21 Oct 2021 15:00:41	U	SMPL
M4287-02 - 1	EXC-SOIL-A	8172	1.6029	-	7471B	PPB	21 Oct 2021 15:02:56	U	SMPL
M4287-06 - 1	EXC-SOIL-B	6718	1.3133	-	7471B	PPB	21 Oct 2021 15:05:12	U	SMPL
M4288-01 - 1	SA-01-101921	3394	0.6514	-	7471B	PPB	21 Oct 2021 15:07:28	U	SMPL
PB140096BL - 1	PBS	-27	-0.0298	-	7471B	PPB	21 Oct 2021 15:12:21	U	SMPL
PB140096BS - 1	LCSS	18762	3.7116	-	7471B	PPB	21 Oct 2021 15:14:37	U	SMPL
M4290-01 - 1	TP-1	2238	0.4212	-	7471B	PPB	21 Oct 2021 15:16:53	U	SMPL
M4290-04 - 1	TH-BS	7133	1.3960	-	7471B	PPB	21 Oct 2021 15:19:10	U	SMPL
M4290-07 - 1	TH-BD	1788	0.3316	-	7471B	PPB	21 Oct 2021 15:21:27	U	SMPL
M4290-10 - 1	TH-BBS	3560	0.6845	-	7471B	PPB	21 Oct 2021 15:23:43	U	SMPL
CCV15 - 1	CCV15	23595	4.6740	-	7471B	PPB	21 Oct 2021 15:25:58	U	SMPL
CCB15 - 1	CCB15	104	-0.0037	-	7471B	PPB	21 Oct 2021 15:28:14	U	SMPL
M4290-13 - 1	TH-BBD	1491	0.2725	-	7471B	PPB	21 Oct 2021 15:30:29	U	SMPL
M4294-01 - 1	WC-2-FS	12877	2.5397	-	7471B	PPB	21 Oct 2021 15:32:44	U	SMPL
M4294-04 - 1	WC-2-ES	31344	6.2170	-	7471B	PPB	21 Oct 2021 15:35:00	U	SMPL
M4294-07 - 1	WC-2-GS	232665	46.3054	-	7471B	PPB	21 Oct 2021 15:37:16	U	SMPL
M4294-10 - 1	WC-2-GD	4823	0.9360	-	7471B	PPB	21 Oct 2021 15:49:31	U	SMPL
M4294-13 - 1	WC-2-HS	31167	6.1818	-	7471B	PPB	21 Oct 2021 15:51:47	U	SMPL
M4294-13DUP - 1	WC-2-HSDUP	28543	5.6593	-	7471B	PPB	21 Oct 2021 15:54:03	U	SMPL
M4294-13MS - 1	WC-2-HSMS	48164	9.5663	-	7471B	PPB	21 Oct 2021 15:59:04	U	SMPL
M4294-13MSD - 1	WC-2-HMSD	48298	9.5930	-	7471B	PPB	21 Oct 2021 16:01:21	U	SMPL
M4295-01 - 1	RBR-251386	5149	1.0009	-	7471B	PPB	21 Oct 2021 16:03:38	U	SMPL
CCV16 - 1	CCV16	24652	4.8845	-	7471B	PPB	21 Oct 2021 16:05:55	U	SMPL
CCB16 - 1	CCB16	86	-0.0073	-	7471B	PPB	21 Oct 2021 16:08:10	U	SMPL
M4297-01 - 1	TR-04-10212021	2100	0.3938	-	7471B	PPB	21 Oct 2021 16:10:26	U	SMPL
M4298-01 - 1	NB-08-102021	1606	0.2954	-	7471B	PPB	21 Oct 2021 16:12:42	U	SMPL
M4300-01 - 1	TH-CS	7093	1.3880	-	7471B	PPB	21 Oct 2021 16:14:58	U	SMPL
M4300-04 - 1	TH-CD	4695	0.9105	-	7471B	PPB	21 Oct 2021 16:17:13	U	SMPL
M4300-07 - 1	TH-CCS	1730	0.3201	-	7471B	PPB	21 Oct 2021 16:19:29	U	SMPL
M4300-10 - 1	TH-CCD	1473	0.2689	-	7471B	PPB	21 Oct 2021 16:21:45	U	SMPL
M4280-07LX5 - 1		439	0.0630	-	7471B	PPB	21 Oct 2021 16:24:02	U	SMPL
M4280-07A - 1		23149	4.5852	-	7471B	PPB	21 Oct 2021 16:26:19	U	SMPL
M4294-13LX5 - 1		6252	1.2205	-	7471B	PPB	21 Oct 2021 16:28:36	U	SMPL
M4294-13A - 1		49456	9.8236	-	7471B	PPB	21 Oct 2021 16:30:52	U	SMPL
CCV17 - 1	CCV17	24283	4.8110	-	7471B	PPB	21 Oct 2021 16:33:08	U	SMPL
CCB17 - 1	CCB17	73	-0.0099	-	7471B	PPB	21 Oct 2021 16:35:26	U	SMPL
M4283-01DLX10 - 1		24986	4.9510	-	7471B	PPB	21 Oct 2021 16:37:44	U	SMPL
M4294-07DLX10 - 1		26679	5.2881	-	7471B	PPB	21 Oct 2021 16:45:04	U	SMPL
CCV18 - 1	CCV18	24560	4.8661	-	7471B	PPB	21 Oct 2021 16:47:20	U	SMPL
CCB18 - 1	CCB18	25	-0.0194	-	7471B	PPB	21 Oct 2021 16:49:36	U	SMPL