


LB117038

7471B

INSTRUMENT ID: CV1

Linear

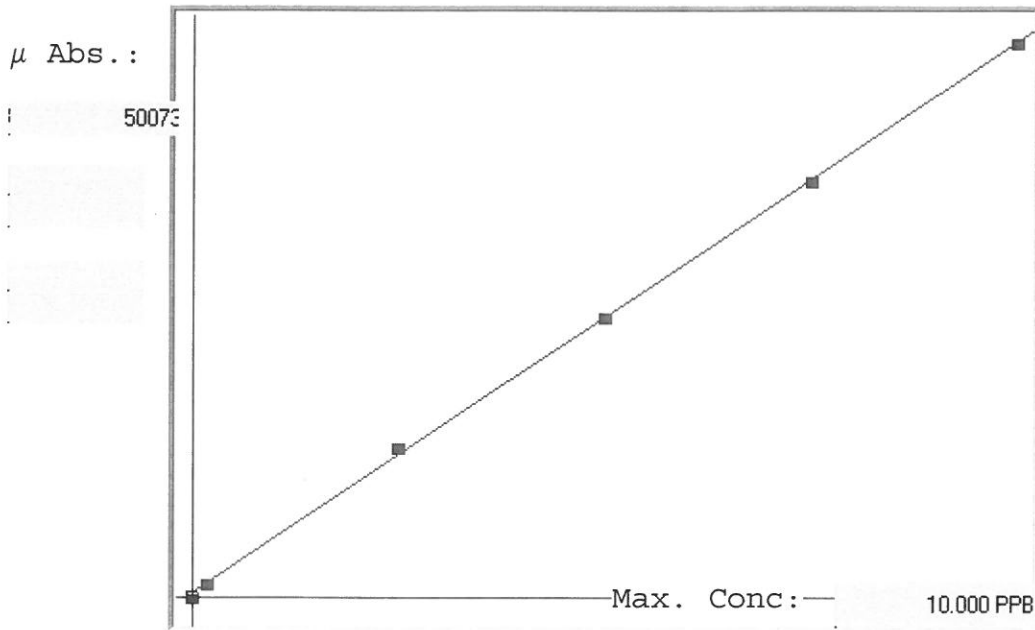

A= 0.0000e+000

B= 2.0085e-004

C= -7.8172e-002

Rho= 0.9998334

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	-0.072	-0.072	31	0.000	31					-14
0.2	0.200	0.172	-0.028	1245	0.0 %	1245					6
2.5	2.500	2.642	0.142	13544	0.0 %	13544					0
5.0	5.000	5.003	0.003	25301	0.0 %	25301					0
7.5	7.500	7.476	-0.024	37609	0.0 %	37609					0
10.0	10.000	9.979	-0.021	50073	0.0 %	50073					0

LB117038 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 27 Oct 2021 08:07:16

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	31	-	0.0000	7471B	PPB	27 Oct 2021 08:14:14	S	Std
0.2 - 1	50.2	1245	-	0.2000	7471B	PPB	27 Oct 2021 08:19:01	S	Std
2.5 - 1	52.5	13544	-	2.5000	7471B	PPB	27 Oct 2021 08:24:07	S	Std
5.0 - 1	55	25301	-	5.0000	7471B	PPB	27 Oct 2021 08:26:25	S	Std
7.5 - 1	57.5	37609	-	7.5000	7471B	PPB	27 Oct 2021 08:28:41	S	Std
10.0 - 1	510	50073	-	10.0000	7471B	PPB	27 Oct 2021 08:36:05	S	Std
ICV59 - 1	ICV59	20303	3.9997	-	7471B	PPB	27 Oct 2021 08:38:51	U	SMPL
ICB59 - 1	ICB59	-79	-0.0940	-	7471B	PPB	27 Oct 2021 08:41:06	U	SMPL
CCV61 - 1	CCV61	24373	4.8171	-	7471B	PPB	27 Oct 2021 08:43:21	U	SMPL
CCB61 - 1	CCB61	-77	-0.0936	-	7471B	PPB	27 Oct 2021 08:45:36	U	SMPL
CRA - 1	CRA	1216	0.1661	-	7471B	PPB	27 Oct 2021 08:47:52	U	SMPL
HighStd - 1	HighStd	50550	10.0747	-	7471B	PPB	27 Oct 2021 08:50:07	U	SMPL
ChkStd - 1	ChkStd	35854	7.1230	-	7471B	PPB	27 Oct 2021 08:52:22	U	SMPL
PB140267BL - 1	PBS	-106	-0.0995	-	7471B	PPB	27 Oct 2021 08:54:39	U	SMPL
PB140267BS - 1	LCSS	21299	4.1997	-	7471B	PPB	27 Oct 2021 08:56:56	U	SMPL
M4336-02 - 1	C1	2625	0.4491	-	7471B	PPB	27 Oct 2021 09:04:03	U	SMPL
M4336-02DUP - 1	C1DUP	2696	0.4633	-	7471B	PPB	27 Oct 2021 09:06:19	U	SMPL
M4336-02MS - 1	C1MS	21753	4.2909	-	7471B	PPB	27 Oct 2021 09:08:36	U	SMPL
M4336-02MSD - 1	C1MSD	23956	4.7334	-	7471B	PPB	27 Oct 2021 09:10:53	U	SMPL
M4336-03 - 1	C2	7275	1.3830	-	7471B	PPB	27 Oct 2021 09:13:08	U	SMPL
CCV62 - 1	CCV62	24356	4.8137	-	7471B	PPB	27 Oct 2021 09:15:24	U	SMPL
CCB62 - 1	CCB62	-55	-0.0892	-	7471B	PPB	27 Oct 2021 09:17:39	U	SMPL
M4336-04 - 1	C3	5362	0.9988	-	7471B	PPB	27 Oct 2021 09:19:55	U	SMPL
M4336-05 - 1	C4	2245	0.3727	-	7471B	PPB	27 Oct 2021 09:22:11	U	SMPL
M4348-02 - 1	354	2098	0.3432	-	7471B	PPB	27 Oct 2021 09:24:26	U	SMPL
M4348-04 - 1	358	3583	0.6415	-	7471B	PPB	27 Oct 2021 09:26:42	U	SMPL
M4348-06 - 1	VNJ-229	3267	0.5780	-	7471B	PPB	27 Oct 2021 09:28:58	U	SMPL
M4348-08 - 1	287	1701	0.2635	-	7471B	PPB	27 Oct 2021 09:31:14	U	SMPL
M4348-10 - 1	370	8033	1.5352	-	7471B	PPB	27 Oct 2021 09:33:30	U	SMPL
M4355-01 - 1	OK-2-102521	1116	0.1460	-	7471B	PPB	27 Oct 2021 09:35:47	U	SMPL
PB140268BL - 1	PBS	17	-0.0748	-	7471B	PPB	27 Oct 2021 09:38:04	U	SMPL
PB140268BS - 1	LCSS	18849	3.7076	-	7471B	PPB	27 Oct 2021 09:40:20	U	SMPL
CCV63 - 1	CCV63	24461	4.8348	-	7471B	PPB	27 Oct 2021 09:42:36	U	SMPL
CCB63 - 1	CCB63	-62	-0.0906	-	7471B	PPB	27 Oct 2021 09:44:51	U	SMPL
M4340-01 - 1	TH-ES	1110	0.1448	-	7471B	PPB	27 Oct 2021 09:47:07	U	SMPL
M4340-01DUP - 1	TH-ESDUP	1021	0.1269	-	7471B	PPB	27 Oct 2021 09:49:22	U	SMPL
M4340-01MS - 1	TH-ESMS	21345	4.2089	-	7471B	PPB	27 Oct 2021 09:51:38	U	SMPL
M4340-01MSD - 1	TH-ESMSD	20917	4.1230	-	7471B	PPB	27 Oct 2021 09:53:53	U	SMPL
M4340-04 - 1	TH-ED	293	-0.0193	-	7471B	PPB	27 Oct 2021 09:56:09	U	SMPL
M4340-07 - 1	TH-EES	1410	0.2050	-	7471B	PPB	27 Oct 2021 09:58:25	U	SMPL
M4340-10 - 1	TH-EED	2709	0.4659	-	7471B	PPB	27 Oct 2021 10:00:41	U	SMPL
M4341-01 - 1	WASTE	2474	0.4187	-	7471B	PPB	27 Oct 2021 10:02:58	U	SMPL
M4343-01 - 1	METRO-SP	2724	0.4689	-	7471B	PPB	27 Oct 2021 10:05:15	U	SMPL
M4356-01 - 1	ETGI-282	1156	0.1540	-	7471B	PPB	27 Oct 2021 10:07:31	U	SMPL
CCV64 - 1	CCV64	25890	5.1218	-	7471B	PPB	27 Oct 2021 10:09:47	U	SMPL
CCB64 - 1	CCB64	-25	-0.0832	-	7471B	PPB	27 Oct 2021 10:12:03	U	SMPL
M4356-03 - 1	VNJ-221	843	0.0911	-	7471B	PPB	27 Oct 2021 10:14:19	U	SMPL
M4357-01 - 1	CL-01-102521	2891	0.5025	-	7471B	PPB	27 Oct 2021 10:16:36	U	SMPL
M4358-01 - 1	TH-FS	450	0.0122	-	7471B	PPB	27 Oct 2021 10:18:52	U	SMPL
M4358-04 - 1	TH-FD	1681	0.2595	-	7471B	PPB	27 Oct 2021 10:21:08	U	SMPL
M4358-07 - 1	TH-GS	2410	0.4059	-	7471B	PPB	27 Oct 2021 10:23:24	U	SMPL
M4358-10 - 1	TH-GD	1001	0.1229	-	7471B	PPB	27 Oct 2021 10:25:40	U	SMPL
M4336-02LX5 - 1		504	0.0231	-	7471B	PPB	27 Oct 2021 10:27:56	U	SMPL
M4336-02A - 1		22954	4.5321	-	7471B	PPB	27 Oct 2021 10:30:13	U	SMPL
M4340-01LX5 - 1		180	-0.0420	-	7471B	PPB	27 Oct 2021 10:51:13	U	SMPL
M4340-01A - 1		21407	4.2214	-	7471B	PPB	27 Oct 2021 10:53:29	U	SMPL
CCV65 - 1	CCV65	24582	4.8591	-	7471B	PPB	27 Oct 2021 10:55:44	U	SMPL
CCB65 - 1	CCB65	-41	-0.0864	-	7471B	PPB	27 Oct 2021 10:58:00	U	SMPL