

LB117092


7470A

INSTRUMENT ID: CV2

Linear

 μ Abs.:

35640

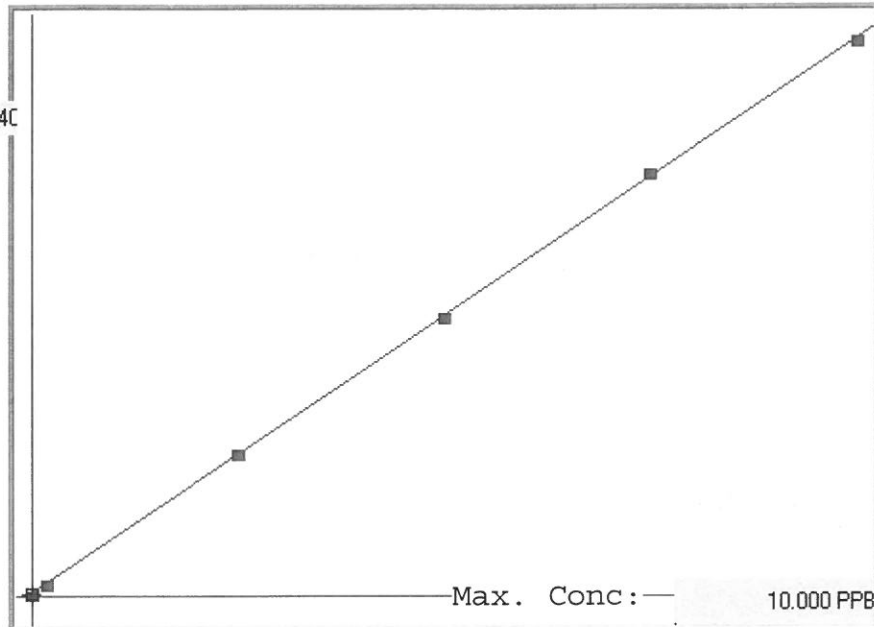

A= 0.0000e+000

B= 2.8049e-004

C= -5.0262e-002

Rho= 0.9999311

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	-0.000	-0.000	178	0.000	178					-
0.2	0.200	0.183	-0.017	833	0.0 %	833					-9
2.5	2.500	2.514	0.014	9143	0.0 %	9143					-1
5.0	5.000	4.972	-0.028	17905	0.0 %	17905					-1
7.5	7.500	7.584	0.084	27219	0.0 %	27219					-1
10.0	10.000	9.946	-0.054	35640	0.0 %	35640					-1

LB117092 INSTRUMENT ID : CV1

Method: 7470A		Operator: Admin		Date of Analysis: 29 Oct 2021 11:43:41					
Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	178	-	0.00007470A		PPB	29 Oct 2021 11:54:50	S	Std
0.2 - 1	50.2	833	-	0.20007470A		PPB	29 Oct 2021 11:57:07	S	Std
2.5 - 1	52.5	9143	-	2.50007470A		PPB	29 Oct 2021 11:59:24	S	Std
5.0 - 1	55	17905	-	5.00007470A		PPB	29 Oct 2021 12:01:40	S	Std
7.5 - 1	57.5	27219	-	7.50007470A		PPB	29 Oct 2021 12:06:36	S	Std
10.0 - 1	510	35640	-	10.00007470A		PPB	29 Oct 2021 12:11:28	S	Std
ICV62 - 1	ICV62	13249	3.6659	-7470A		PPB	29 Oct 2021 12:16:38	U	SMPL
ICB62 - 1	ICB62	145	-0.0096	-7470A		PPB	29 Oct 2021 12:18:53	U	SMPL
CCV78 - 1	CCV78	18631	5.1755	-7470A		PPB	29 Oct 2021 12:21:08	U	SMPL
CCB78 - 1	CCB78	148	-0.0087	-7470A		PPB	29 Oct 2021 12:23:23	U	SMPL
CRA - 1	CRA	803	0.1750	-7470A		PPB	29 Oct 2021 12:25:38	U	SMPL
HighStd - 1	HighStd	35671	9.9551	-7470A		PPB	29 Oct 2021 12:27:53	U	SMPL
ChkStd - 1	ChkStd	26010	7.2453	-7470A		PPB	29 Oct 2021 12:30:08	U	SMPL
PB140320BL - 1	PBW	85	-0.0264	-7470A		PPB	29 Oct 2021 12:35:09	U	SMPL
PB140320BS - 1	LCSW	14552	4.0314	-7470A		PPB	29 Oct 2021 12:37:25	U	SMPL
M4366-03 - 1	1520-1521	45	-0.0376	-7470A		PPB	29 Oct 2021 12:39:42	U	SMPL
M4366-03DUP - 1	1520-1521DUP	68	-0.0312	-7470A		PPB	29 Oct 2021 12:41:59	U	SMPL
M4366-03MS - 1	1520-1521MS	14535	4.0267	-7470A		PPB	29 Oct 2021 12:44:16	U	SMPL
M4366-03MSD - 1	1520-1521MSD	12763	3.5296	-7470A		PPB	29 Oct 2021 12:46:33	U	SMPL
M4378-02 - 1	WASTE-CHAR-(EXCESS)	15	-0.0461	-7470A		PPB	29 Oct 2021 12:48:48	U	SMPL
CCV79 - 1	CCV79	18846	5.2358	-7470A		PPB	29 Oct 2021 12:51:04	U	SMPL
CCB79 - 1	CCB79	163	-0.0045	-7470A		PPB	29 Oct 2021 12:53:19	U	SMPL
M4380-02 - 1	WASTE-CHAR-(SUSPECT)	79	-0.0281	-7470A		PPB	29 Oct 2021 12:55:34	U	SMPL
M4384-01 - 1	COMP-A	85	-0.0264	-7470A		PPB	29 Oct 2021 12:57:49	U	SMPL
M4384-02 - 1	COMP-B	103	-0.0214	-7470A		PPB	29 Oct 2021 13:00:05	U	SMPL
M4384-03 - 1	COMP-C	118	-0.0172	-7470A		PPB	29 Oct 2021 13:02:20	U	SMPL
M4384-04 - 1	1890	325	0.0409	-7470A		PPB	29 Oct 2021 13:04:36	U	SMPL
PB140321BL - 1	PBW	68	-0.0312	-7470A		PPB	29 Oct 2021 13:06:52	U	SMPL
PB140321BS - 1	LCSW	15745	4.3660	-7470A		PPB	29 Oct 2021 13:09:09	U	SMPL
M4384-05 - 1	COMP-TOTE	269	0.0252	-7470A		PPB	29 Oct 2021 13:11:26	U	SMPL
M4384-06 - 1	1900	60	-0.0334	-7470A		PPB	29 Oct 2021 13:13:43	U	SMPL
M4390-02 - 1	FRAC-COMP	107	-0.0202	-7470A		PPB	29 Oct 2021 13:15:59	U	SMPL
CCV80 - 1	CCV80	18027	5.0061	-7470A		PPB	29 Oct 2021 13:18:14	U	SMPL
CCB80 - 1	CCB80	113	-0.0186	-7470A		PPB	29 Oct 2021 13:20:30	U	SMPL
M4390-02DUP - 1	FRAC-COMPDUP	90	-0.0250	-7470A		PPB	29 Oct 2021 13:22:45	U	SMPL
M4390-02MS - 1	FRAC-COMPMS	14781	4.0957	-7470A		PPB	29 Oct 2021 13:25:01	U	SMPL
M4390-02MSD - 1	FRAC-COMPMSD	14113	3.9083	-7470A		PPB	29 Oct 2021 13:30:24	U	SMPL
PB140322BL - 1	PBW	51	-0.0360	-7470A		PPB	29 Oct 2021 13:32:40	U	SMPL
PB140322BS - 1	LCSW	12996	3.5950	-7470A		PPB	29 Oct 2021 13:34:55	U	SMPL
M4372-15 - 1	GW-1	75	-0.0292	-7470A		PPB	29 Oct 2021 13:37:11	U	SMPL
M4372-15DUP - 1	GW-1DUP	164	-0.0043	-7470A		PPB	29 Oct 2021 13:39:28	U	SMPL
M4372-15MS - 1	GW-1MS	14750	4.0870	-7470A		PPB	29 Oct 2021 13:41:44	U	SMPL
M4372-15MSD - 1	GW-1MSD	14252	3.9473	-7470A		PPB	29 Oct 2021 13:44:01	U	SMPL
M4385-01 - 1	T2229-2232	7	-0.0483	-7470A		PPB	29 Oct 2021 13:46:17	U	SMPL
CCV81 - 1	CCV81	18192	5.0524	-7470A		PPB	29 Oct 2021 13:48:32	U	SMPL
CCB81 - 1	CCB81	61	-0.0332	-7470A		PPB	29 Oct 2021 13:50:48	U	SMPL
M4390-01 - 1	FRAC-COMP	97	-0.0231	-7470A		PPB	29 Oct 2021 13:53:03	U	SMPL
M4392-01 - 1	N41924	47	-0.0371	-7470A		PPB	29 Oct 2021 13:55:19	U	SMPL
PB140320TB - 1	PB140291TB	-8	-0.0525	-7470A		PPB	29 Oct 2021 13:57:35	U	SMPL
PB140321TB - 1	PB140300TB	9	-0.0477	-7470A		PPB	29 Oct 2021 13:59:50	U	SMPL
M4366-03LX5 - 1		26	-0.0430	-7470A		PPB	29 Oct 2021 14:02:07	U	SMPL
M4366-03A - 1		12486	3.4519	-7470A		PPB	29 Oct 2021 14:11:34	U	SMPL
M4390-02LX5 - 1		-27	-0.0578	-7470A		PPB	29 Oct 2021 14:13:51	U	SMPL
M4390-02A - 1		13033	3.6054	-7470A		PPB	29 Oct 2021 14:16:07	U	SMPL
M4372-15LX5 - 1		-3	-0.0511	-7470A		PPB	29 Oct 2021 14:18:24	U	SMPL
M4372-15A - 1		14116	3.9091	-7470A		PPB	29 Oct 2021 14:20:40	U	SMPL
CCV82 - 1	CCV82	16744	4.6463	-7470A		PPB	29 Oct 2021 14:22:56	U	SMPL
CCB82 - 1	CCB82	133	-0.0130	-7470A		PPB	29 Oct 2021 14:25:11	U	SMPL