


LB117128

7470A

INSTRUMENT ID: CV1

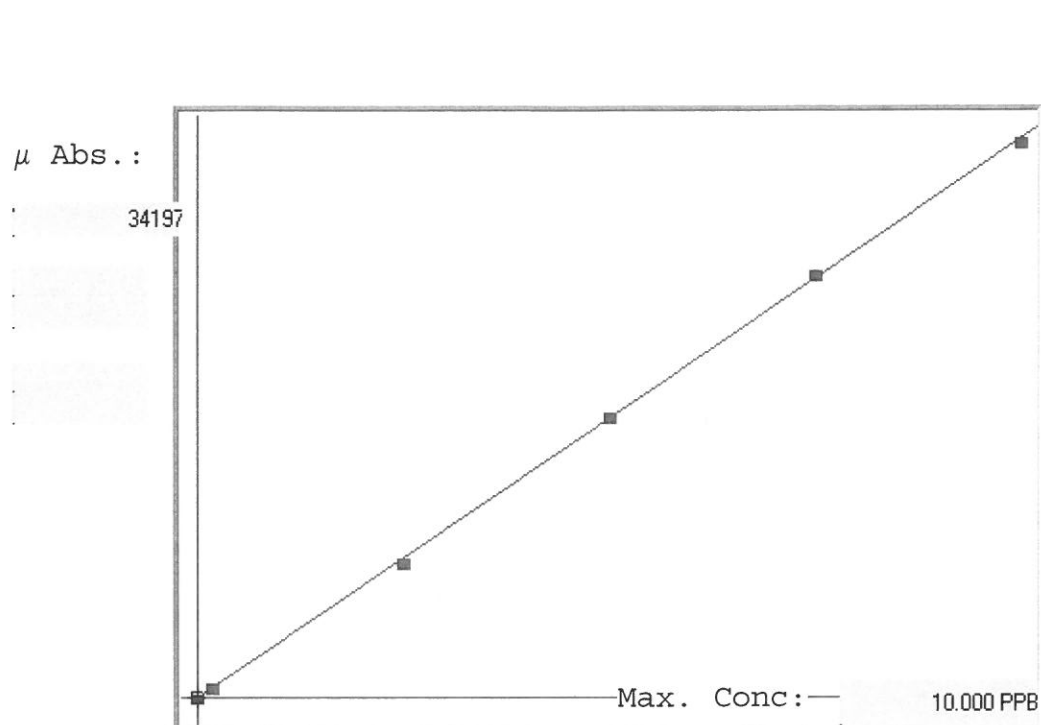

Linear

A= 0.0000e+000

B= 2.8993e-004

C= 1.2580e-002

Rho= 0.9998702

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	900
0.0	0.000	0.018	0.018	17	0.000	17					-
0.2	0.200	0.198	-0.002	639	0.0 %	639					-1
2.5	2.500	2.426	-0.074	8324	0.0 %	8324					-3
5.0	5.000	5.038	0.038	17332	0.0 %	17332					1
7.5	7.500	7.593	0.093	26147	0.0 %	26147					1
10.0	10.000	9.927	-0.073	34197	0.0 %	34197					-1

LB117128 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 02 Nov 2021 10:53:05

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	17	-	0.0000	7470A	PPB	02 Nov 2021 11:06:23	S	Std
0.2 - 1	50.2	639	-	0.2000	7470A	PPB	02 Nov 2021 11:08:39	S	Std
2.5 - 1	50.5	8324	-	2.5000	7470A	PPB	02 Nov 2021 11:10:56	S	Std
5.0 - 1	55	17332	-	5.0000	7470A	PPB	02 Nov 2021 11:13:13	S	Std
7.5 - 1	57.5	26147	-	7.5000	7470A	PPB	02 Nov 2021 11:15:30	S	Std
10.0 - 1	510	34197	-	10.0000	7470A	PPB	02 Nov 2021 11:20:19	S	Std
ICV64 - 1	ICV64	14132	4.1099	-	7470A	PPB	02 Nov 2021 11:22:58	U	SMPL
ICB64 - 1	ICB64	45	0.0256	-	7470A	PPB	02 Nov 2021 11:25:13	U	SMPL
CCV86 - 1	CCV86	17555	5.1024	-	7470A	PPB	02 Nov 2021 11:27:28	U	SMPL
CCB86 - 1	CCB86	25	0.0198	-	7470A	PPB	02 Nov 2021 11:29:43	U	SMPL
CRA - 1	CRA	595	0.1851	-	7470A	PPB	02 Nov 2021 11:31:58	U	SMPL
HighStd - 1	HighStd	34473	10.0075	-	7470A	PPB	02 Nov 2021 11:34:13	U	SMPL
ChkStd - 1	ChkStd	24254	7.0446	-	7470A	PPB	02 Nov 2021 11:36:28	U	SMPL
PB140363BL - 1	PBW	-103	-0.0173	-	7470A	PPB	02 Nov 2021 11:38:45	U	SMPL
PB140363BS - 1	LCSW	14752	4.2897	-	7470A	PPB	02 Nov 2021 11:41:01	U	SMPL
M4395-02 - 1	MH-FFS	-33	0.0030	-	7470A	PPB	02 Nov 2021 11:43:17	U	SMPL
M4395-05 - 1	MH-FFD	22	0.0190	-	7470A	PPB	02 Nov 2021 11:45:33	U	SMPL
M4395-08 - 1	MH-GGS	15	0.0169	-	7470A	PPB	02 Nov 2021 11:47:50	U	SMPL
M4395-11 - 1	MH-GGD	16	0.0172	-	7470A	PPB	02 Nov 2021 11:50:07	U	SMPL
M4406-02 - 1	CHRT-20310	17	0.0175	-	7470A	PPB	02 Nov 2021 11:52:22	U	SMPL
CCV87 - 1	CCV87	16868	4.9032	-	7470A	PPB	02 Nov 2021 11:54:38	U	SMPL
CCB87 - 1	CCB87	8	0.0149	-	7470A	PPB	02 Nov 2021 11:56:53	U	SMPL
M4406-02DUP - 1	CHRT-20310DUP	11	0.0158	-	7470A	PPB	02 Nov 2021 11:59:08	U	SMPL
M4406-02MS - 1	CHRT-20310MS	13041	3.7936	-	7470A	PPB	02 Nov 2021 12:01:23	U	SMPL
M4406-02MSD - 1	CHRT-20310MSD	13152	3.8258	-	7470A	PPB	02 Nov 2021 12:03:39	U	SMPL
PB140363TB - 1	PB140326TB	-54	-0.0031	-	7470A	PPB	02 Nov 2021 12:05:55	U	SMPL
M4406-02LX5 - 1		22	0.0190	-	7470A	PPB	02 Nov 2021 12:08:10	U	SMPL
M4406-02A - 1		13903	4.0435	-	7470A	PPB	02 Nov 2021 12:10:27	U	SMPL
CCV88 - 1	CCV88	16595	4.8240	-	7470A	PPB	02 Nov 2021 12:12:44	U	SMPL
CCB88 - 1	CCB88	17	0.0175	-	7470A	PPB	02 Nov 2021 12:15:00	U	SMPL