

12117151

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : AM Instrument ID : Konelab

11/3/2021 12:36

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	94.051	0.0	0.067	
ICB1	-0.143	0.0	0.001	
CCV1	238.545	0.0	0.170	
CCB1	-0.099	0.0	0.001	
PB140463BL	0.015	0.0	0.001	
M4411-02	-0.372	0.0	0.000	
M4411-02DUP	-0.319	0.0	0.000	
M4411-05	-0.368	0.0	0.000	
M4470-02	-0.266	0.0	0.000	
M4470-05	-0.115	0.0	0.001	
M4470-08	-0.308	0.0	0.000	
M4472-02	-0.236	0.0	0.000	
M4472-05	-0.135	0.0	0.001	
M4472-08	-0.073	0.0	0.001	
CCV2	240.367	0.0	0.171	
CCB2	0.191	0.0	0.001	

N	16
Mean	35.671
SD	82.9327
CV%	232.49

Aquakem v. 7.2AQ1

Results from time period:

Wed Nov 03 10:31:41 2021

Wed Nov 03 12:00:52 2021

Sample Id	Sam/Ctr/c	Test short nar	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Reactive CN	P	0.9902	µg/l	11/3/2021 11:29:05	
5.OPPBCN	A	Reactive CN	P	5.3888	µg/l	11/3/2021 11:29:06	
10PPBCN	A	Reactive CN	P	10.3153	µg/l	11/3/2021 11:29:07	
50PPBCN	A	Reactive CN	P	48.1876	µg/l	11/3/2021 11:29:08	
100PPBCN	A	Reactive CN	P	99.946	µg/l	11/3/2021 11:29:09	
250PPBCN	A	Reactive CN	P	249.9804	µg/l	11/3/2021 11:29:10	
500PPBCN	A	Reactive CN	P	500.1916	µg/l	11/3/2021 11:29:11	
ICV1	S	Reactive CN	P	94.051	µg/l	11/3/2021 11:53:37	
ICB1	S	Reactive CN	P	-0.1432	µg/l	11/3/2021 11:53:38	
CCV1	S	Reactive CN	P	238.5447	µg/l	11/3/2021 11:53:41	
CCB1	S	Reactive CN	P	-0.0987	µg/l	11/3/2021 11:53:42	
PB140463BL	S	Reactive CN	P	0.0154	µg/l	11/3/2021 11:53:45	
M4411-02	S	Reactive CN	P	-0.3723	µg/l	11/3/2021 11:53:46	
M4411-02DUP	S	Reactive CN	P	-0.3187	µg/l	11/3/2021 12:00:43	
M4411-05	S	Reactive CN	P	-0.3684	µg/l	11/3/2021 12:00:44	
M4470-02	S	Reactive CN	P	-0.2659	µg/l	11/3/2021 12:00:45	
M4470-05	S	Reactive CN	P	-0.1153	µg/l	11/3/2021 12:00:46	
M4470-08	S	Reactive CN	P	-0.3082	µg/l	11/3/2021 12:00:47	
M4472-02	S	Reactive CN	P	-0.2358	µg/l	11/3/2021 12:00:48	
M4472-05	S	Reactive CN	P	-0.1351	µg/l	11/3/2021 12:00:49	
M4472-08	S	Reactive CN	P	-0.0728	µg/l	11/3/2021 12:00:50	
CCV2	S	Reactive CN	P	240.3671	µg/l	11/3/2021 12:00:51	
CCB2	S	Reactive CN	P	0.1913	µg/l	11/3/2021 12:00:52	

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : AK

Instrument ID : Konelab

11/3/2021 11:30


Test Total CN

Accepted 11/3/2021 11:30

Factor 1411
Bias 0.001

Coeff. of det. 0.999978

Errors

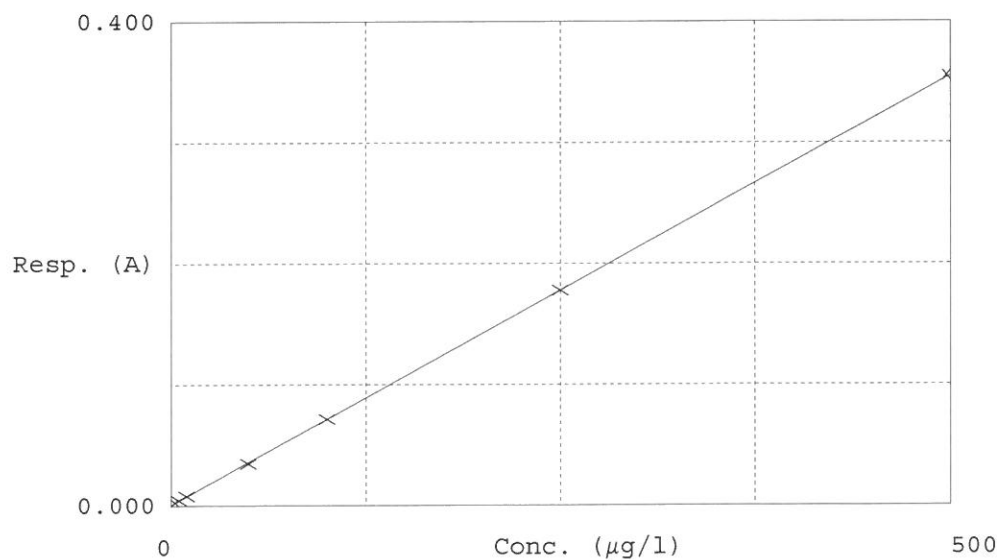

	Calibrator	Response	Calc. con.	Conc.	Rel. Errors	
1	0.0PPBCN	0.001	0.9902	0.0000	7.8	
2	5.0PPBCN	0.004	5.3888	5.0000	3.2	
3	10PPBCN	0.008	10.3153	10.0000	-3.6	
4	50PPBCN	0.035	48.1876	50.0000	-0.1	AB
5	100PPBCN	0.072	99.9460	100.0000	0.0	
6	250PPBCN	0.178	249.9804	250.0000	0.0	
7	500PPBCN	0.355	500.1916	500.0000	0.0	11/03/21