

LB117236

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : AL Instrument ID : Konelab

11/8/2021 14:30

Test: Phenolics- mg/L

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	0.993	0.0	0.095	
ICB1	0.003	0.0	0.005	
CCV1	1.000	0.0	0.095	
CCB1	0.002	0.0	0.005	
PB140578BL	0.003	0.0	0.005	
PB140578BS	1.003	0.0	0.095	
M4068-03	0.026	0.0	0.008	
PB140579BL	0.001	0.0	0.005	
PB140579BS	1.003	0.0	0.095	
M4068-09	0.027	0.0	0.008	
CCV2	1.009	0.0	0.096	
CCB2	0.003	0.0	0.005	

N	12
Mean	0.423
SD	0.5110
CV%	120.83

Aquakem v. 7.2AQ1

Results from time period:

Mon Nov 08 14:18:17 2021

Mon Nov 08 14:28:30 2021

Sample Id	Sam/Ctr/c	Test short	Test type	Result	Result unit	Result date and time	Stat
0.00PPM	A	Phenolics-	P	0.0017	mg/l	11/8/2021 11:42:45	
0.05PPM	A	Phenolics-	P	0.0516	mg/l	11/8/2021 11:42:46	
0.1PPM	A	Phenolics-	P	0.1041	mg/l	11/8/2021 11:42:47	
0.25PPM	A	Phenolics-	P	0.2543	mg/l	11/8/2021 11:42:48	
0.50PPM	A	Phenolics-	P	0.5008	mg/l	11/8/2021 11:42:49	
1.0PPM	A	Phenolics-	P	0.977	mg/l	11/8/2021 11:42:50	
2.0PPM	A	Phenolics-	P	2.0105	mg/l	11/8/2021 11:42:51	
ICV1	S	Phenolics-	P	0.9928	mg/l	11/8/2021 14:18:18	
ICB1	S	Phenolics-	P	0.0034	mg/l	11/8/2021 14:18:19	
CCV1	S	Phenolics-	P	1.0001	mg/l	11/8/2021 14:18:22	
CCB1	S	Phenolics-	P	0.0025	mg/l	11/8/2021 14:18:23	
PB140578BL	S	Phenolics-	P	0.0031	mg/l	11/8/2021 14:18:25	
PB140578BS	S	Phenolics-	P	1.0034	mg/l	11/8/2021 14:18:28	
M4068-03	S	Phenolics-	P	0.0262	mg/l	11/8/2021 14:28:20	
PB140579BL	S	Phenolics-	P	0.0014	mg/l	11/8/2021 14:28:22	
PB140579BS	S	Phenolics-	P	1.0028	mg/l	11/8/2021 14:28:24	
M4068-09	S	Phenolics-	P	0.0266	mg/l	11/8/2021 14:28:25	
CCV2	S	Phenolics-	P	1.0094	mg/l	11/8/2021 14:28:27	
CCB2	S	Phenolics-	P	0.0033	mg/l	11/8/2021 14:28:29	

CHEMTECH CONSULTING GROUP INC

284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : AB

Instrument ID : Konelab

11/8/2021 11:44

Test Phenolics-


Accepted 11/8/2021 11:44

Factor 11.11

Bias 0.005

Coeff. of det. 0.999783

Errors

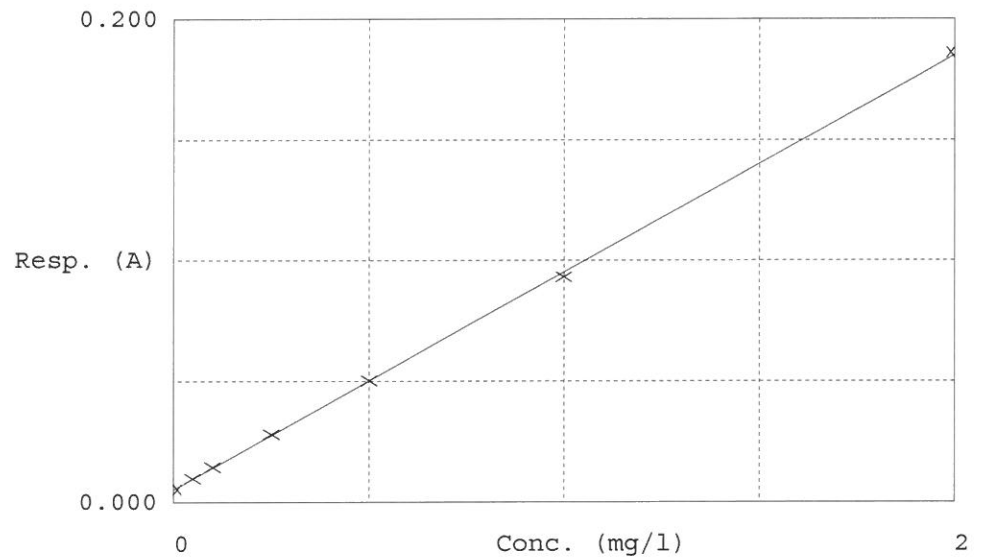

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.00PPM	0.005	0.0017	0.0000	
2	Phenol-2	0.010	0.0516	0.0500	
3	Phenol-2	0.015	0.1041	0.1000	
4	Phenol-2	0.028	0.2543	0.2500	
5	Phenol-2	0.050	0.5008	0.5000	
6	Phenol-2	0.093	0.9770	1.0000	
7	Phenol-2	0.186	2.0105	2.0000	

p.c.
Errors3.2
4.1
1.2
0.2
-2.3
0.5AB
11/8/21