


LB 117282

7470A

INSTRUMENT ID: CV1

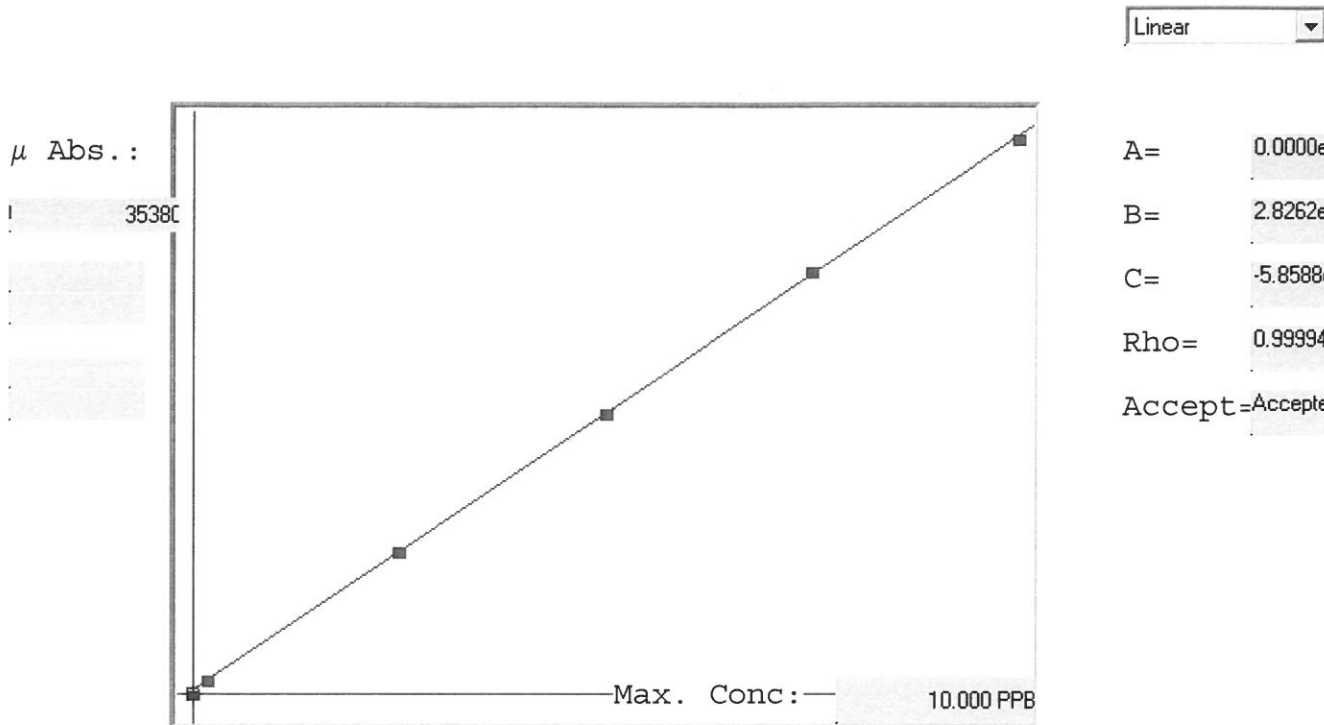

A= 0.0000e+000

B= 2.8262e-004

C= -5.8588e-002

Rho= 0.9999419

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	-0.035	-0.035	85	0.000	85					-
0.2	0.200	0.204	0.004	929	0.0 %	929					2
2.5	2.500	2.513	0.013	9099	0.0 %	9099					1
5.0	5.000	5.010	0.010	17936	0.0 %	17936					0
7.5	7.500	7.567	0.067	26981	0.0 %	26981					1
10.0	10.000	9.940	-0.060	35380	0.0 %	35380					-1

LB117282 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 10 Nov 2021 08:41:29

Sample ID	Extended ID	μ Abs	Conc	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	85	-	0.0000	7470A	PPB	10 Nov 2021 08:57:18	S	Std
0.2 - 1	50-2	929	-	0.2000	7470A	PPB	10 Nov 2021 09:04:52	S	Std
2.5 - 1	52-5	9099	-	2.5000	7470A	PPB	10 Nov 2021 09:07:09	S	Std
5.0 - 1	55	17936	-	5.0000	7470A	PPB	10 Nov 2021 09:09:26	S	Std
7.5 - 1	57-5	26981	-	7.5000	7470A	PPB	10 Nov 2021 09:14:14	S	Std
10.0 - 1	510	35380	-	10.0000	7470A	PPB	10 Nov 2021 09:19:02	S	Std
ICV75 - 1	ICV75	14246	3.9676	-	7470A	PPB	10 Nov 2021 09:21:40	U	SMPL
ICB75 - 1	ICB75	100	-0.0303	-	7470A	PPB	10 Nov 2021 09:26:37	U	SMPL
CCV36 - 1	CCV36	17016	4.7504	-	7470A	PPB	10 Nov 2021 09:28:52	U	SMPL
CCB36 - 1	CCB36	48	-0.0450	-	7470A	PPB	10 Nov 2021 09:31:07	U	SMPL
CRA - 1	CRA	857	0.1836	-	7470A	PPB	10 Nov 2021 09:33:22	U	SMPL
HighStd - 1	HighStd	33321	9.3585	-	7470A	PPB	10 Nov 2021 09:35:37	U	SMPL
ChkStd - 1	ChkStd	25618	7.1815	-	7470A	PPB	10 Nov 2021 09:40:25	U	SMPL
PB140640BL - 1	PBW	67	-0.0397	-	7470A	PPB	10 Nov 2021 09:47:43	U	SMPL
PB140640BS - 1	LCSW	12869	3.5784	-	7470A	PPB	10 Nov 2021 09:50:00	U	SMPL
M4454-14 - 1	30859	-45	-0.0713	-	7470A	PPB	10 Nov 2021 09:55:23	U	SMPL
M4454-15 - 1	30858	35	-0.0487	-	7470A	PPB	10 Nov 2021 09:57:40	U	SMPL
M4454-13 - 1	30860-OIL	28	-0.0507	-	7470A	PPB	10 Nov 2021 10:00:12	U	SMPL
M4454-16 - 1	11221-A	58	-0.0422	-	7470A	PPB	10 Nov 2021 10:02:45	U	SMPL
M4454-16DUP - 1	11221-ADUP	45	-0.0459	-	7470A	PPB	10 Nov 2021 10:05:01	U	SMPL
CCV37 - 1	CCV37	17866	4.9907	-	7470A	PPB	10 Nov 2021 10:07:16	U	SMPL
CCB37 - 1	CCB37	92	-0.0326	-	7470A	PPB	10 Nov 2021 10:09:32	U	SMPL
M4454-16MS - 1	11221-AMS	14329	3.9911	-	7470A	PPB	10 Nov 2021 10:11:47	U	SMPL
M4454-16MSD - 1	11221-AMSD	14141	3.9379	-	7470A	PPB	10 Nov 2021 10:14:02	U	SMPL
M4454-17 - 1	33104	-24	-0.0654	-	7470A	PPB	10 Nov 2021 10:16:18	U	SMPL
PB140641BL - 1	PBW	163	-0.0125	-	7470A	PPB	10 Nov 2021 10:18:34	U	SMPL
PB140641BS - 1	LCSW	13179	3.6660	-	7470A	PPB	10 Nov 2021 10:20:50	U	SMPL
M4068-07 - 1	LOD-MDL-WATER-01-QT4-2021	359	0.0429	-	7470A	PPB	10 Nov 2021 10:28:10	U	SMPL
M4068-08 - 1	LOQ-WATER-02-QT4-2021	909	0.1983	-	7470A	PPB	10 Nov 2021 10:30:26	U	SMPL
M4600-01 - 1	FM786-N34145	24	-0.0518	-	7470A	PPB	10 Nov 2021 10:32:43	U	SMPL
M4600-01DUP - 1	FM786-N34145DUP	37	-0.0481	-	7470A	PPB	10 Nov 2021 10:35:00	U	SMPL
M4600-01MS - 1	FM786-N34145MS	13723	3.8198	-	7470A	PPB	10 Nov 2021 10:37:16	U	SMPL
CCV38 - 1	CCV38	17490	4.8844	-	7470A	PPB	10 Nov 2021 10:39:31	U	SMPL
CCB38 - 1	CCB38	41	-0.0470	-	7470A	PPB	10 Nov 2021 10:41:47	U	SMPL
M4600-01MSD - 1	FM786-N34145MSD	13422	3.7347	-	7470A	PPB	10 Nov 2021 10:44:03	U	SMPL
PB140640TB - 1	PB140606TB	-33	-0.0679	-	7470A	PPB	10 Nov 2021 10:46:19	U	SMPL
M4454-16LX5 - 1		21	-0.0527	-	7470A	PPB	10 Nov 2021 10:48:37	U	SMPL
M4454-16A - 1		14603	4.0685	-	7470A	PPB	10 Nov 2021 10:50:53	U	SMPL
M4600-01LX5 - 1		-32	-0.0676	-	7470A	PPB	10 Nov 2021 10:53:10	U	SMPL
M4600-01A - 1		13521	3.7627	-	7470A	PPB	10 Nov 2021 10:55:27	U	SMPL
CCV39 - 1	CCV39	17572	4.9076	-	7470A	PPB	10 Nov 2021 10:57:43	U	SMPL
CCB39 - 1	CCB39	55	-0.0430	-	7470A	PPB	10 Nov 2021 11:00:00	U	SMPL