

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : RA

Instrument ID : Konelab

11/10/2021 9:43

Reactive
Test: ~~Total~~ CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	96.270	0.0	0.067	
ICB1	1.219	0.0	0.001	
CCV1	244.441	0.0	0.170	
CCB1	0.940	0.0	0.001	
PB140659BL	0.876	0.0	0.001	
M4587-01	0.889	0.0	0.001	
M4587-01DUP	1.034	0.0	0.001	
M4593-02	1.125	0.0	0.001	
M4595-03	1.103	0.0	0.001	
M4595-04	1.074	0.0	0.001	
M4595-07	1.071	0.0	0.001	
M4595-08	1.923	0.0	0.001	
M4601-02	0.932	0.0	0.001	
M4603-02	1.805	0.0	0.001	
CCV2	245.983	0.0	0.171	
CCB2	1.285	0.0	0.001	
M4567-01	1.128	0.0	0.001	
M4567-01DUP	1.045	0.0	0.001	
M4567-02	1.053	0.0	0.001	
M4600-01	1.420	0.0	0.001	
CCV3	248.775	0.0	0.173	
CCB3	1.251	0.0	0.001	

N	22
Mean	38.938
SD	86.7636
CV%	222.82

Aquakem v. 7.2AQ1

Results from time period:

Wed Nov 10 08:37:44 2021

Wed Nov 10 09:42:32 2021

Sample Id	Sam/Ctr/c/	Test short na	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Reactive CN	P	0.9434	µg/l	11/10/2021 8:55:00	
5.OPPBCN	A	Reactive CN	P	6.0381	µg/l	11/10/2021 8:55:01	
10PPBCN	A	Reactive CN	P	10.6835	µg/l	11/10/2021 8:55:02	
50PPBCN	A	Reactive CN	P	47.6222	µg/l	11/10/2021 8:55:03	
100PPBCN	A	Reactive CN	P	99.0143	µg/l	11/10/2021 8:55:04	
250PPBCN	A	Reactive CN	P	250.575	µg/l	11/10/2021 8:55:05	
500PPBCN	A	Reactive CN	P	500.1234	µg/l	11/10/2021 8:55:06	
ICV1	S	Reactive CN	P	96.2697	µg/l	11/10/2021 9:27:44	
ICB1	S	Reactive CN	P	1.2192	µg/l	11/10/2021 9:27:47	
CCV1	S	Reactive CN	P	244.441	µg/l	11/10/2021 9:27:49	
CCB1	S	Reactive CN	P	0.9396	µg/l	11/10/2021 9:27:51	
PB140659BL	S	Reactive CN	P	0.8755	µg/l	11/10/2021 9:27:52	
M4587-01	S	Reactive CN	P	0.8891	µg/l	11/10/2021 9:27:54	
M4587-01DUP	S	Reactive CN	P	1.0344	µg/l	11/10/2021 9:35:16	
M4593-02	S	Reactive CN	P	1.125	µg/l	11/10/2021 9:35:17	
M4595-03	S	Reactive CN	P	1.1029	µg/l	11/10/2021 9:35:18	
M4595-04	S	Reactive CN	P	1.0739	µg/l	11/10/2021 9:35:19	
M4595-07	S	Reactive CN	P	1.0709	µg/l	11/10/2021 9:35:20	
M4595-08	S	Reactive CN	P	1.9234	µg/l	11/10/2021 9:35:21	
M4601-02	S	Reactive CN	P	0.932	µg/l	11/10/2021 9:35:22	
M4603-02	S	Reactive CN	P	1.8047	µg/l	11/10/2021 9:35:23	
CCV2	S	Reactive CN	P	245.9833	µg/l	11/10/2021 9:35:24	
CCB2	S	Reactive CN	P	1.2855	µg/l	11/10/2021 9:35:25	
M4567-01	S	Reactive CN	P	1.1277	µg/l	11/10/2021 9:35:26	
M4567-01DUP	S	Reactive CN	P	1.0454	µg/l	11/10/2021 9:42:23	
M4567-02	S	Reactive CN	P	1.0532	µg/l	11/10/2021 9:42:24	
M4600-01	S	Reactive CN	P	1.42	µg/l	11/10/2021 9:42:25	
CCV3	S	Reactive CN	P	248.7752	µg/l	11/10/2021 9:42:26	
CCB3	S	Reactive CN	P	1.2509	µg/l	11/10/2021 9:42:27	

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

11/10/2021 8:56 Reviewed by : pl Instrument ID : Konelab


Test Total CN

Accepted 11/10/2021 8:56

Factor 1435
Bias 0

Coeff. of det. 0.999954

Errors

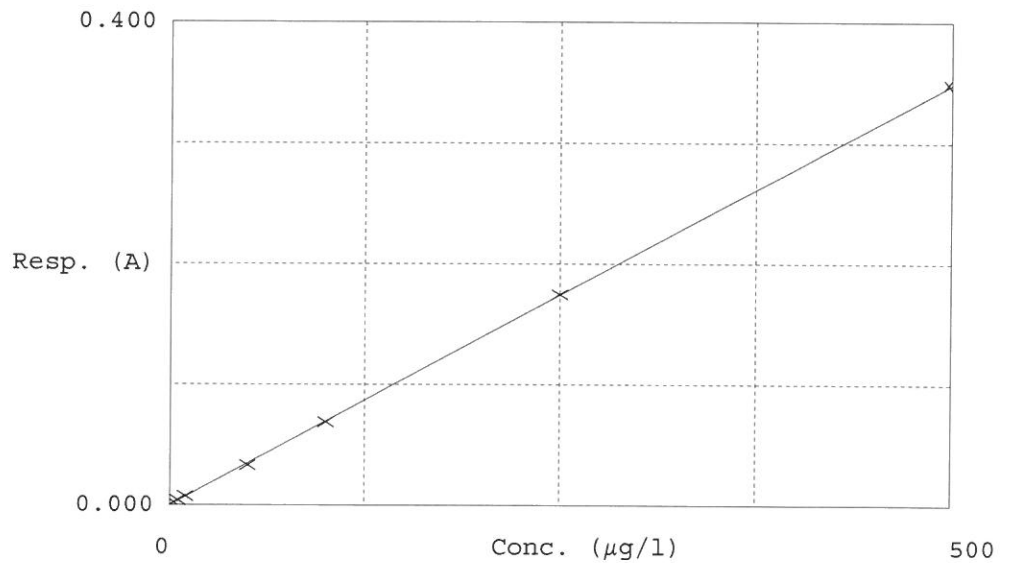

	Calibrator	Response	Calc. con.	Conc.	Rel. Errors
1	0.0PPBCN	0.001	0.9434	0.0000	
2	5.0PPBCN	0.004	6.0381	5.0000	20.8
3	10PPBCN	0.007	10.6835	10.0000	6.8
4	50PPBCN	0.033	47.6222	50.0000	-4.8
5	100PPBCN	0.069	99.0143	100.0000	-1.0
6	250PPBCN	0.175	250.5750	250.0000	0.2
7	500PPBCN	0.348	500.1234	500.0000	0.0

AB
11/10/21