

LB117379

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092Reviewed by : AS

Instrument ID : Konelab

11/15/2021 11:49

Test: ^{negative}
~~Total~~ CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	96.268	0.0	0.067	
ICB1	1.021	0.0	0.001	
CCV1	245.246	0.0	0.171	
CCB1	0.994	0.0	0.001	
PB140738BL	0.836	0.0	0.001	
M4640-02	0.938	0.0	0.001	
M4640-02DUP	1.148	0.0	0.001	
M4644-02	0.654	0.0	0.001	
M4656-02	0.879	0.0	0.001	
M4656-03	0.916	0.0	0.001	
M4656-04	0.769	0.0	0.001	
M4656-05	0.877	0.0	0.001	
M4693-04	0.743	0.0	0.001	
M4656-01	1.107	0.0	0.001	
CCV2	244.036	0.0	0.170	
CCB2	1.157	0.0	0.001	
M4693-02	0.931	0.0	0.001	
PB140739BL	1.085	0.0	0.001	
M4656-06	0.801	0.0	0.001	
M4656-06DUP	0.907	0.0	0.001	
M4656-07	0.818	0.0	0.001	
M4656-08	0.921	0.0	0.001	
M4656-09	0.816	0.0	0.001	
M4660-01	0.983	0.0	0.001	
M4674-09	1.074	0.0	0.001	
CCV3	249.807	0.0	0.174	
CCB3	1.181	0.0	0.001	

N	27
Mean	31.737
SD	79.4680
CV%	250.39

Aquakem v. 7.2AQ1

Results from time period:

Mon Nov 15 11:29:48 2021

Mon Nov 15 11:44:07 2021

Sample Id	Sam/Ctr/c	Test short name	Test type	Result	Result unit	Result date and time
0.OPPBCN	A	Reactive CN	P	0.68	µg/l	11/15/2021 10:03:10
5.OPPBCN	A	Reactive CN	P	5.4167	µg/l	11/15/2021 10:03:11
10PPBCN	A	Reactive CN	P	9.988	µg/l	11/15/2021 10:03:12
50PPBCN	A	Reactive CN	P	47.8871	µg/l	11/15/2021 10:03:13
100PPBCN	A	Reactive CN	P	98.4627	µg/l	11/15/2021 10:03:14
250PPBCN	A	Reactive CN	P	254.1014	µg/l	11/15/2021 10:03:15
500PPBCN	A	Reactive CN	P	498.4641	µg/l	11/15/2021 10:03:16
ICV1	S	Reactive CN	P	96.2679	µg/l	11/15/2021 11:29:48
ICB1	S	Reactive CN	P	1.0209	µg/l	11/15/2021 11:29:50
CCV1	S	Reactive CN	P	245.2456	µg/l	11/15/2021 11:29:52
CCB1	S	Reactive CN	P	0.9939	µg/l	11/15/2021 11:29:55
PB140738BL	S	Reactive CN	P	0.8357	µg/l	11/15/2021 11:29:56
M4640-02	S	Reactive CN	P	0.9378	µg/l	11/15/2021 11:29:57
M4640-02DUP	S	Reactive CN	P	1.1477	µg/l	11/15/2021 11:29:58
M4644-02	S	Reactive CN	P	0.6537	µg/l	11/15/2021 11:37:20
M4656-02	S	Reactive CN	P	0.879	µg/l	11/15/2021 11:37:21
M4656-03	S	Reactive CN	P	0.9162	µg/l	11/15/2021 11:37:22
M4656-04	S	Reactive CN	P	0.7689	µg/l	11/15/2021 11:37:23
M4656-05	S	Reactive CN	P	0.877	µg/l	11/15/2021 11:37:24
M4693-04	S	Reactive CN	P	0.7425	µg/l	11/15/2021 11:37:25
M4656-01	S	Reactive CN	P	1.1066	µg/l	11/15/2021 11:37:26
CCV2	S	Reactive CN	P	244.0357	µg/l	11/15/2021 11:37:27
CCB2	S	Reactive CN	P	1.1566	µg/l	11/15/2021 11:37:28
M4693-02	S	Reactive CN	P	0.9307	µg/l	11/15/2021 11:37:29
PB140739BL	S	Reactive CN	P	1.0855	µg/l	11/15/2021 11:37:30
M4656-06	S	Reactive CN	P	0.8011	µg/l	11/15/2021 11:43:59
M4656-06DUP	S	Reactive CN	P	0.9065	µg/l	11/15/2021 11:44:00
M4656-07	S	Reactive CN	P	0.8178	µg/l	11/15/2021 11:44:01
M4656-08	S	Reactive CN	P	0.9206	µg/l	11/15/2021 11:44:02
M4656-09	S	Reactive CN	P	0.8163	µg/l	11/15/2021 11:44:03
M4660-01	S	Reactive CN	P	0.9831	µg/l	11/15/2021 11:44:04
M4674-09	S	Reactive CN	P	1.0741	µg/l	11/15/2021 11:44:05
CCV3	S	Reactive CN	P	249.807	µg/l	11/15/2021 11:44:06
CCB3	S	Reactive CN	P	1.1815	µg/l	11/15/2021 11:44:07

CHEMTECH CONSULTING GROUP INC

284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : RA

Instrument ID : Konelab

11/15/2021 10:04

Test Total CN


Accepted 11/15/2021 10:04

Factor 1437

Bias 0

Coeff. of det. 0.999870

Errors

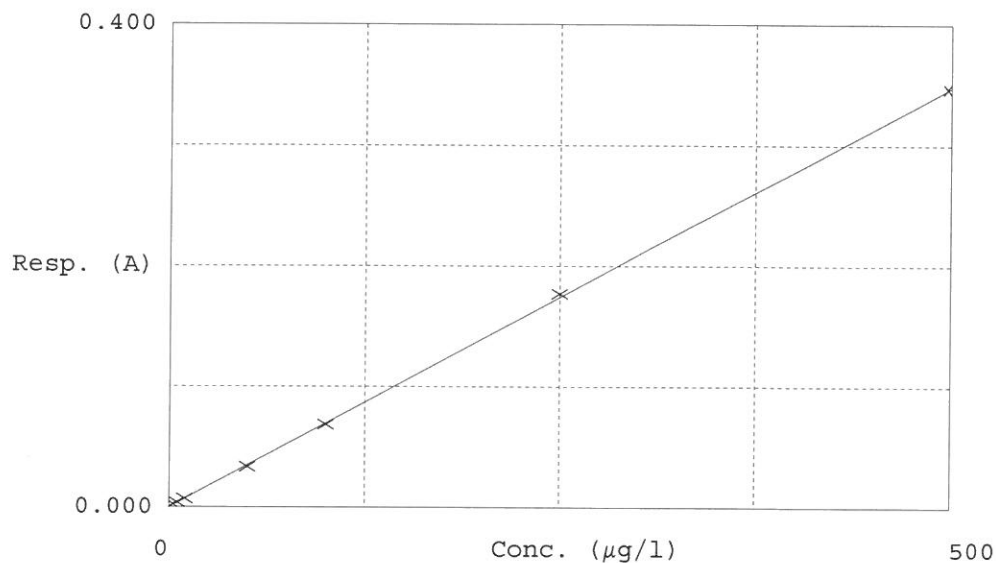

	Calibrator	Response	Calc. con.	Conc.	Rel. Errors
1	0.0PPBCN	0.001	0.6800	0.0000	-
2	5.0PPBCN	0.004	5.4167	5.0000	-8.3
3	10PPBCN	0.007	9.9880	10.0000	-0.1
4	50PPBCN	0.033	47.8871	50.0000	-4.2
5	100PPBCN	0.069	98.4627	100.0000	-1.5
6	250PPBCN	0.177	254.1014	250.0000	1.6
7	500PPBCN	0.347	498.4641	500.0000	-0.3

RB
11/15/21