

LB117380

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC

284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : MA Instrument ID : Konelab

11/15/2021 12:34

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	96.251	0.0	0.067	
ICB1	1.100	0.0	0.001	
CCV1	247.432	0.0	0.172	
CCB1	0.786	0.0	0.001	
PB140753BL	0.927	0.0	0.001	
PB140753BS	97.409	0.0	0.068	
MIDPB140753	242.985	0.0	0.169	
M4692-02	0.916	0.0	0.001	
M4692-02DUP	0.875	0.0	0.001	
M4692-02MS	37.184	0.0	0.026	
M4692-02MSD	37.338	0.0	0.026	
CCV2	256.846	0.0	0.179	
CCB2	0.970	0.0	0.001	

N	13
Mean	78.540
SD	103.1092
CV%	131.28

99.7% (90-110)
11/15/21

Aquakem v. 7.2AQ1

Results from time period:

Mon Nov 15 12:14:15 2021

Mon Nov 15 12:26:09 2021

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Total CN	P	0.68	µg/l	11/15/2021 10:03:10	
5.OPPBCN	A	Total CN	P	5.4167	µg/l	11/15/2021 10:03:11	
10PPBCN	A	Total CN	P	9.988	µg/l	11/15/2021 10:03:12	
50PPBCN	A	Total CN	P	47.8871	µg/l	11/15/2021 10:03:13	
100PPBCN	A	Total CN	P	98.4627	µg/l	11/15/2021 10:03:14	
250PPBCN	A	Total CN	P	254.1014	µg/l	11/15/2021 10:03:15	
500PPBCN	A	Total CN	P	498.4641	µg/l	11/15/2021 10:03:16	
ICV1	S	Total CN	P	96.2508	µg/l	11/15/2021 12:14:15	
ICB1	S	Total CN	P	1.1003	µg/l	11/15/2021 12:14:17	
CCV1	S	Total CN	P	247.432	µg/l	11/15/2021 12:14:20	
CCB1	S	Total CN	P	0.7855	µg/l	11/15/2021 12:14:22	
PB140753BL	S	Total CN	P	0.9271	µg/l	11/15/2021 12:14:24	
PB140753BS	S	Total CN	P	97.4092	µg/l	11/15/2021 12:14:25	
MIDPB140753	S	Total CN	P	242.9846	µg/l	11/15/2021 12:21:49	
M4692-02	S	Total CN	P	0.9164	µg/l	11/15/2021 12:21:51	
M4692-02DUP	S	Total CN	P	0.8749	µg/l	11/15/2021 12:21:53	
M4692-02MS	S	Total CN	P	37.1841	µg/l	11/15/2021 12:21:54	
M4692-02MSD	S	Total CN	P	37.3378	µg/l	11/15/2021 12:21:56	
CCV2	S	Total CN	P	256.8457	µg/l	11/15/2021 12:26:07	
CCB2	S	Total CN	P	0.9695	µg/l	11/15/2021 12:26:09	

CHEMTECH CONSULTING GROUP INC

284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : RA

Instrument ID : Konelab

11/15/2021 10:04

Test Total CN


Accepted 11/15/2021 10:04

Factor 1437

Bias 0

Coeff. of det. 0.999870

Errors

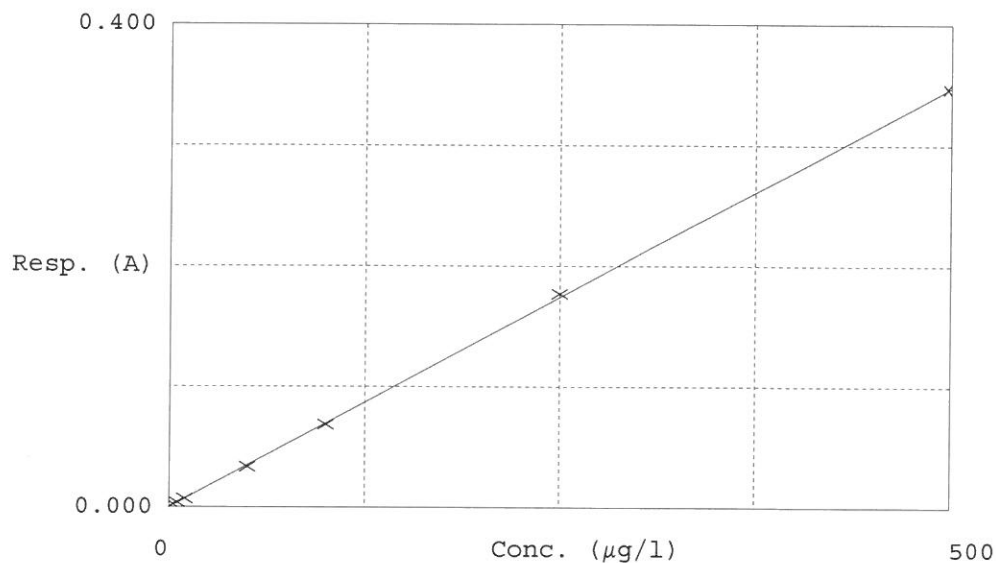

	Calibrator	Response	Calc. con.	Conc.	Rel. Errors
1	0.0PPBCN	0.001	0.6800	0.0000	-
2	5.0PPBCN	0.004	5.4167	5.0000	8.3
3	10PPBCN	0.007	9.9880	10.0000	-0.1
4	50PPBCN	0.033	47.8871	50.0000	-4.2
5	100PPBCN	0.069	98.4627	100.0000	-1.5
6	250PPBCN	0.177	254.1014	250.0000	1.6
7	500PPBCN	0.347	498.4641	500.0000	-0.3

RB 11/15/21