

CHEMTECH CONSULTING GROUP INC

284 Sheffield Street, Mountainside, NJ 07092

11/15/2021 12:57

Reviewed by : AD Instrument ID : Konelab

Test CNEPA-NEW

Accepted

11/15/2021 12:57

Factor Slope

.1093 0.000915

Bias y-intercept


0.006

AD
11/15/21

Coeff. of det.

0.999976

Errors

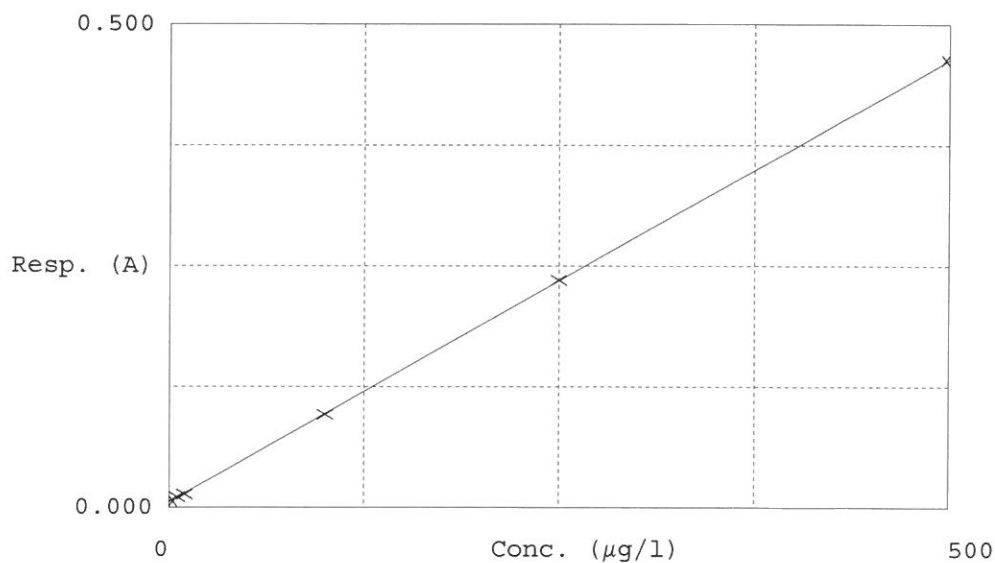

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.006	0.7700	0.0000	15.2
2	5.0PPBCN	0.011	5.9085	5.0000	-12.5
3	10PPBCN	0.014	8.7474	10.0000	-1.0
4	100PPBCN	0.096	98.9618	100.0000	0.3
5	250PPBCN	0.235	250.7775	250.0000	0.2
6	500PPBCN	0.463	499.8349	500.0000	

AD

11/15/21

03117387

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC

284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : AS

Instrument ID : Konelab

11/15/2021 14:05

Test: CNEPA-NEW

Sample Id	Result	Dil. 1 +	Response	Errors
ICV001 ICV001	94.738	0.0	0.092	
ICB001 ICB001	1.733	0.0	0.007	
CCV001 CCV001	241.527	0.0	0.227	
CCB001 CCB001	1.787	0.0	0.007	
PB140698BL	1.623	0.0	0.007	
M4608-01	2.551	0.0	0.008	
M4608-03	1.555	0.0	0.007	
M4608-06	1.982	0.0	0.008	
M4641-02	1.648	0.0	0.007	
M4676-01	1.495	0.0	0.007	
M4676-01DUP	1.966	0.0	0.008	
M4676-07	3.190	0.0	0.009	
M4676-09	3.893	0.0	0.009	
M4676-03MS	95.863	0.0	0.094	
M4676-03MSD	94.067	0.0	0.092	
CCV002 CCV002	257.722	0.0	0.242	
CCB002 CCB002	1.478	0.0	0.007	

N	17
Mean	47.578
SD	84.1673
CV%	176.91

M4676-04
AS
11/28/21
Not
Used
AS
11/28/21

Aquakem v. 7.2AQ1

Results from time period:

Mon Nov 15 12:56:46 2021

Mon Nov 15 14:01:54 2021

Sample Id	Sam/Ctr/c/	Test sho	Test type	Result	Result unit	Result date and time	Stat
S0	A	CNEPA-I P		0.77	µg/l	11/15/2021 12:56:46	
S5.0	A	CNEPA-I P		5.9085	µg/l	11/15/2021 12:56:47	
S10.0	A	CNEPA-I P		8.7474	µg/l	11/15/2021 12:56:48	
S100.0	A	CNEPA-I P		98.9618	µg/l	11/15/2021 12:56:49	
S250.0	A	CNEPA-I P		250.7775	µg/l	11/15/2021 12:56:50	
S500.0	A	CNEPA-I P		499.8349	µg/l	11/15/2021 12:56:51	
ICV001 ICV001	S	CNEPA-I P		94.7383	µg/l	11/15/2021 13:50:55	
ICB001 ICB001	S	CNEPA-I P		1.7334	µg/l	11/15/2021 13:50:57	
CCV001 CCV001	S	CNEPA-I P		241.527	µg/l	11/15/2021 13:51:00	
CCB001 CCB001	S	CNEPA-I P		1.7873	µg/l	11/15/2021 13:51:02	
PB140698BL	S	CNEPA-I P		1.6226	µg/l	11/15/2021 13:51:03	
M4608-01	S	CNEPA-I P		2.5507	µg/l	11/15/2021 13:51:05	
M4608-03	S	CNEPA-I P		1.555	µg/l	11/15/2021 13:58:30	
M4608-06	S	CNEPA-I P		1.9818	µg/l	11/15/2021 13:58:31	
M4641-02	S	CNEPA-I P		1.6476	µg/l	11/15/2021 13:58:32	
M4676-01	S	CNEPA-I P		1.495	µg/l	11/15/2021 13:58:33	
M4676-01DUP	S	CNEPA-I P		1.9661	µg/l	11/15/2021 13:58:34	
M4676-07	S	CNEPA-I P		3.1899	µg/l	11/15/2021 13:58:37	
M4676-09	S	CNEPA-I P		3.8931	µg/l	11/15/2021 13:58:38	
M4676-03MS	S	CNEPA-I P		95.8628	µg/l	11/15/2021 13:58:39	
M4676-03MSD	S	CNEPA-I P		94.0672	µg/l	11/15/2021 13:58:40	
CCV002 CCV002	S	CNEPA-I P		257.7223	µg/l	11/15/2021 14:01:53	
CCB002 CCB002	S	CNEPA-I P		1.4782	µg/l	11/15/2021 14:01:54	

Not Used
AB
11/20/21