

LB117397

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : pb

Instrument ID : Konelab

11/16/2021 14:25

Test: Phenolics-

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	1.045	0.0	0.096	
ICB1	-0.011	0.0	0.005	
CCV1	1.054	0.0	0.097	
CCB1	-0.006	0.0	0.005	
PB140742BL	-0.006	0.0	0.006	
PB140742BS	1.050	0.0	0.097	
M4608-01	-0.007	0.0	0.005	
M4608-03	-0.004	0.0	0.006	
M4608-06	-0.003	0.0	0.006	
M4641-02	0.172	0.0	0.021	
M4676-01	0.042	0.0	0.010	
M4676-01DUP	0.040	0.0	0.010	
M4676-03MS	1.171	0.0	0.107	
M4676-04MSD	1.175	0.0	0.108	
M4676-07	-0.004	0.0	0.006	
M4676-09	-0.003	0.0	0.006	
CCV2	1.058	0.0	0.097	
CCB2	0.002	0.0	0.006	

N	18
Mean	0.376
SD	0.5240
CV%	139.39

Aquakem v. 7.2AQ1

Results from time period:

Tue Nov 16 13:17:47 2021

Tue Nov 16 14:24:37 2021

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.00PPM	A	Phenolics-	P	-0.0019	mg/l	11/16/2021 13:17:47	
0.05PPM	A	Phenolics-	P	0.049	mg/l	11/16/2021 13:17:48	
0.1PPM	A	Phenolics-	P	0.102	mg/l	11/16/2021 13:17:49	
0.25PPM	A	Phenolics-	P	0.2514	mg/l	11/16/2021 13:17:50	
0.50PPM	A	Phenolics-	P	0.499	mg/l	11/16/2021 13:17:51	
1.0PPM	A	Phenolics-	P	1.001	mg/l	11/16/2021 13:17:52	
2.0PPM	A	Phenolics-	P	1.9995	mg/l	11/16/2021 13:17:53	
ICV1	S	Phenolics-	P	1.0451	mg/l	11/16/2021 14:18:42	
ICB1	S	Phenolics-	P	-0.011	mg/l	11/16/2021 14:18:43	
CCV1	S	Phenolics-	P	1.054	mg/l	11/16/2021 14:18:44	
CCB1	S	Phenolics-	P	-0.006	mg/l	11/16/2021 14:18:45	
PB140742BL	S	Phenolics-	P	-0.0059	mg/l	11/16/2021 14:18:46	
PB140742BS	S	Phenolics-	P	1.0505	mg/l	11/16/2021 14:18:47	
M4608-01	S	Phenolics-	P	-0.0071	mg/l	11/16/2021 14:18:48	
M4608-03	S	Phenolics-	P	-0.0045	mg/l	11/16/2021 14:18:49	
M4608-06	S	Phenolics-	P	-0.0032	mg/l	11/16/2021 14:18:50	
M4641-02	S	Phenolics-	P	0.1724	mg/l	11/16/2021 14:18:51	
M4676-01	S	Phenolics-	P	0.0418	mg/l	11/16/2021 14:18:52	
M4676-01DUP	S	Phenolics-	P	0.0404	mg/l	11/16/2021 14:18:53	
M4676-03MS	S	Phenolics-	P	1.1715	mg/l	11/16/2021 14:24:32	
M4676-04MSD	S	Phenolics-	P	1.1746	mg/l	11/16/2021 14:24:33	
M4676-07	S	Phenolics-	P	-0.0039	mg/l	11/16/2021 14:24:34	
M4676-09	S	Phenolics-	P	-0.0025	mg/l	11/16/2021 14:24:35	
CCV2	S	Phenolics-	P	1.0576	mg/l	11/16/2021 14:24:36	
CCB2	S	Phenolics-	P	0.0023	mg/l	11/16/2021 14:24:37	

CHEMTECH CONSULTING GROUP INC

284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : RB

Instrument ID : Konelab

11/16/2021 13:18

Test Phenolics-


Accepted 11/16/2021 13:18

Factor 11.57

Bias 0.006

Coeff. of det. 0.999996

Errors

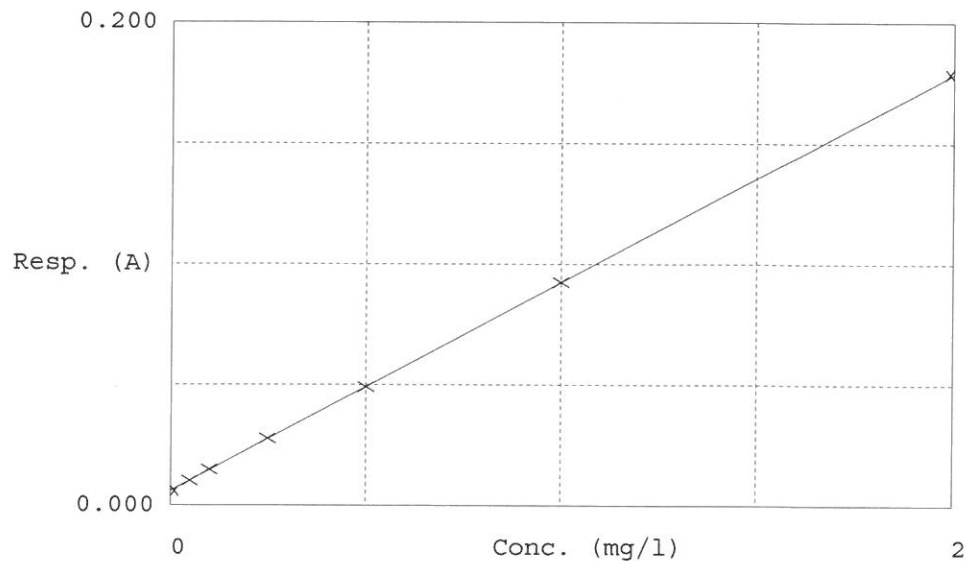

	Calibrator	Response	Calc. con.	Conc.	Rel. Errors
1	0.00PPM	0.006	-0.0019	0.0000	-2.0
2	Phenol-2	0.010	0.0490	0.0500	2.0
3	Phenol-2	0.015	0.1020	0.1000	0.6
4	Phenol-2	0.028	0.2514	0.2500	0.2
5	Phenol-2	0.049	0.4990	0.5000	0.1
6	Phenol-2	0.093	1.0010	1.0000	0.0
7	Phenol-2	0.179	1.9995	2.0000	0.0

RB
11/16/21