

LB117448

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : AL

Instrument ID : Konelab

11/18/2021 11:38

Test: ~~Total~~ ^{Residue} CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	95.841	0.0	0.077	
ICB1	-0.131	0.0	0.001	
CCV1	244.014	0.0	0.195	
CCB1	-0.076	0.0	0.001	
PB140865BL	-0.320	0.0	0.001	
M4700-02	-0.221	0.0	0.001	
M4700-02DUP	-0.386	0.0	0.001	
M4729-01	-0.465	0.0	0.001	
M4731-02	-0.508	0.0	0.001	
M4736-02	-0.398	0.0	0.001	
CCV2	254.961	0.0	0.204	
CCB2	0.266	0.0	0.001	

N	12
Mean	49.381
SD	97.4549
CV%	197.35

Aquakem v. 7.2AQ1

Results from time period:

Thu Nov 18 09:55:02 2021

Thu Nov 18 11:38:22 2021

Sample Id	Sam/Ctr/c	Test short nam	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Reactive CN	P	-0.4548	µg/l	11/18/2021 11:01:46	
5.OPPBCN	A	Reactive CN	P	4.5464	µg/l	11/18/2021 11:01:47	
10PPBCN	A	Reactive CN	P	9.4221	µg/l	11/18/2021 11:01:48	
50PPBCN	A	Reactive CN	P	49.845	µg/l	11/18/2021 11:01:49	
100PPBCN	A	Reactive CN	P	100.7823	µg/l	11/18/2021 11:01:50	
250PPBCN	A	Reactive CN	P	251.9676	µg/l	11/18/2021 11:01:51	
500PPBCN	A	Reactive CN	P	498.8913	µg/l	11/18/2021 11:01:52	
ICV1	S	Reactive CN	P	95.8414	µg/l	11/18/2021 11:33:32	
ICB1	S	Reactive CN	P	-0.1307	µg/l	11/18/2021 11:33:34	
CCV1	S	Reactive CN	P	244.0136	µg/l	11/18/2021 11:33:35	
CCB1	S	Reactive CN	P	-0.0757	µg/l	11/18/2021 11:33:37	
PB140865BL	S	Reactive CN	P	-0.3203	µg/l	11/18/2021 11:33:39	
M4700-02	S	Reactive CN	P	-0.221	µg/l	11/18/2021 11:33:40	
M4700-02DUP	S	Reactive CN	P	-0.3864	µg/l	11/18/2021 11:33:41	
M4729-01	S	Reactive CN	P	-0.4652	µg/l	11/18/2021 11:38:18	
M4731-02	S	Reactive CN	P	-0.5081	µg/l	11/18/2021 11:38:19	
M4736-02	S	Reactive CN	P	-0.3977	µg/l	11/18/2021 11:38:20	
CCV2	S	Reactive CN	P	254.961	µg/l	11/18/2021 11:38:21	
CCB2	S	Reactive CN	P	0.2659	µg/l	11/18/2021 11:38:22	

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : AB

Instrument ID : Konelab

11/18/2021 11:05


Test Total CN

Accepted 11/18/2021 11:05

Factor 1255
Bias 0.001

Coeff. of det. 0.999968

Errors

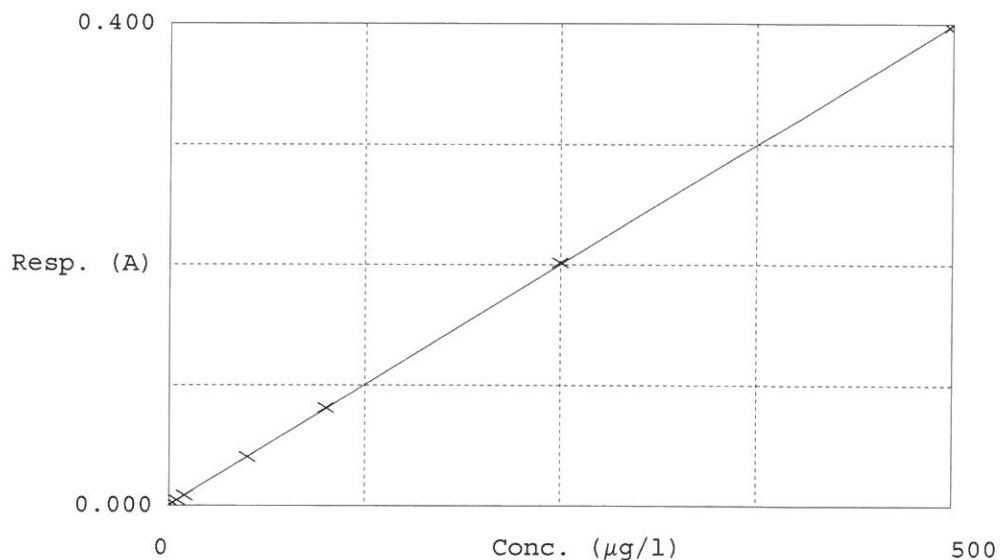

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.001	-0.4548	0.0000	
2	5.0PPBCN	0.005	4.5464	5.0000	
3	10PPBCN	0.008	9.4221	10.0000	
4	50PPBCN	0.041	49.8450	50.0000	
5	100PPBCN	0.081	100.7823	100.0000	
6	250PPBCN	0.202	251.9676	250.0000	
7	500PPBCN	0.398	498.8913	500.0000	

Rel.

Errors

-9.1
-5.8
-0.3
0.8
0.8
-0.2

AB
11/18/21