


LB117429

7471B

INSTRUMENT ID: CV2

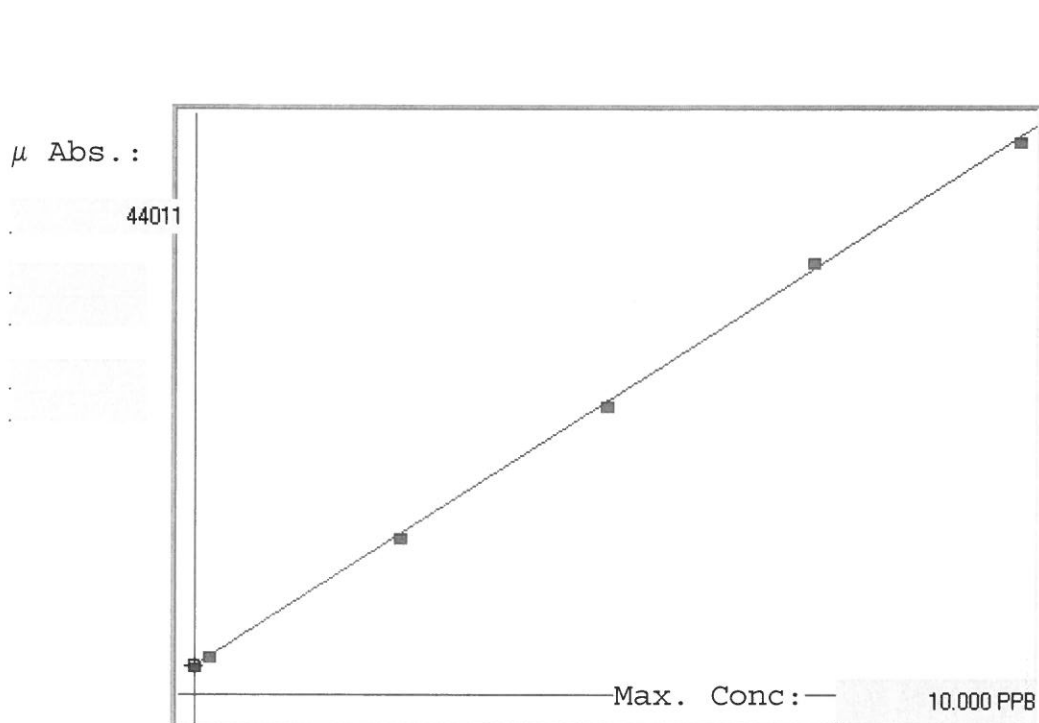

Linear

A= 0.0000e+000

B= 2.3737e-004

C= -5.3307e-001

Rho= 0.9997653

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%ob
0.0	0.000	0.013	0.013	2300	0.000	2300					3
0.2	0.200	0.207	0.007	3117	0.0 %	3117					-1
2.5	2.500	2.465	-0.035	12630	0.0 %	12630					-1
5.0	5.000	4.941	-0.059	23061	0.0 %	23061					-1
7.5	7.500	7.661	0.161	34521	0.0 %	34521					2
10.0	10.000	9.914	-0.086	44011	0.0 %	44011					-1

LB117489 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 22 Nov 2021 14:34:29

Sample ID	Extended ID	μ Abs.	Conc.	Std. Conc	Method	Units	Date	Type	Type
0.0 - 1	50	2300	-	0.0000	7471B	PPB	22 Nov 2021 14:37:52	S	Std
0.2 - 1	50.2	3117	-	0.2000	7471B	PPB	22 Nov 2021 14:40:10	S	Std
2.5 - 1	52.1	12630	-	2.5000	7471B	PPB	22 Nov 2021 14:42:27	S	Std
5.0 - 1	55	23061	-	5.0000	7471B	PPB	22 Nov 2021 14:44:44	S	Std
7.5 - 1	57.5	34521	-	7.5000	7471B	PPB	22 Nov 2021 14:51:11	S	Std
10.0 - 1	510	44011	-	10.0000	7471B	PPB	22 Nov 2021 14:56:05	S	Std
ICV89 - 1	ICV89	20389	4.3066	-	7471B	PPB	22 Nov 2021 14:58:49	U	SMPL
ICB89 - 1	ICB89	2317	0.0169	-	7471B	PPB	22 Nov 2021 15:03:57	U	SMPL
CCV01 - 1	CCV01	23081	4.9456	-	7471B	PPB	22 Nov 2021 15:06:12	U	SMPL
CCB01 - 1	CCB01	2119	-0.0301	-	7471B	PPB	22 Nov 2021 15:08:27	U	SMPL
CRA - 1	CRA	3231	0.2339	-	7471B	PPB	22 Nov 2021 15:10:43	U	SMPL
HighStd - 1	HighStd	44748	10.0886	-	7471B	PPB	22 Nov 2021 15:12:59	U	SMPL
ChkStd - 1	ChkStd	32121	7.0914	-	7471B	PPB	22 Nov 2021 15:15:14	U	SMPL
PB140954BL - 1	PBS	2298	0.0124	-	7471B	PPB	22 Nov 2021 15:20:04	U	SMPL
PB140954BS - 1	LCSS	17729	3.6752	-	7471B	PPB	22 Nov 2021 15:22:19	U	SMPL
M4754-01 - 1	TP-4-COMP	3668	0.3376	-	7471B	PPB	22 Nov 2021 15:24:36	U	SMPL
M4776-01 - 1	RO-72-11948	9006	1.6046	-	7471B	PPB	22 Nov 2021 15:26:53	U	SMPL
M4781-01 - 1	ETGI-354	3381	0.2695	-	7471B	PPB	22 Nov 2021 15:29:10	U	SMPL
M4782-01 - 1	CL-02-111921	4885	0.6265	-	7471B	PPB	22 Nov 2021 15:31:26	U	SMPL
M4783-01 - 1	RBR-200033	4365	0.5030	-	7471B	PPB	22 Nov 2021 15:33:42	U	SMPL
CCV02 - 1	CCV02	22994	4.9249	-	7471B	PPB	22 Nov 2021 15:35:57	U	SMPL
CCB02 - 1	CCB02	2091	-0.0367	-	7471B	PPB	22 Nov 2021 15:38:12	U	SMPL
M4786-01 - 1	RO-279	3655	0.3345	-	7471B	PPB	22 Nov 2021 15:40:28	U	SMPL
M4786-03 - 1	RO-357	3608	0.3233	-	7471B	PPB	22 Nov 2021 15:42:43	U	SMPL
M4796-01 - 1	EO-03-111921	12209	2.3649	-	7471B	PPB	22 Nov 2021 15:44:58	U	SMPL
M4801-01 - 1	SITE-1-DRILL-CUTTINGS-20211119	1950	-0.0702	-	7471B	PPB	22 Nov 2021 15:47:14	U	SMPL
M4801-01DUP - 1	SITE-1-DRILL-CUTTINGS-20211119DUP	2040	-0.0488	-	7471B	PPB	22 Nov 2021 15:49:30	U	SMPL
M4801-01MS - 1	SITE-1-DRILL-CUTTINGS-20211119MS	21031	4.4590	-	7471B	PPB	22 Nov 2021 15:51:47	U	SMPL
M4801-01MSD - 1	SITE-1-DRILL-CUTTINGS-20211119MSD	21079	4.4704	-	7471B	PPB	22 Nov 2021 15:54:03	U	SMPL
M4801-01LX5 - 1		2183	-0.0149	-	7471B	PPB	22 Nov 2021 15:56:21	U	SMPL
M4801-01A - 1		21018	4.4559	-	7471B	PPB	22 Nov 2021 15:58:38	U	SMPL
CCV03 - 1	CCV03	22680	4.8504	-	7471B	PPB	22 Nov 2021 16:00:53	U	SMPL
CCB03 - 1	CCB03	2091	-0.0367	-	7471B	PPB	22 Nov 2021 16:03:09	U	SMPL