

LB 117528

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092Reviewed by : 12 Instrument ID : Konelab

11/24/2021 13:51

Test: CNEPA-NEW

Sample Id	Result <i>µg/L</i>	Dil. 1 +	Response	Errors
ICV001 ICV001	94.059	0.0	0.105	
ICB001 ICB001	0.488	0.0	0.008	
CCV001 CCV001	242.047	0.0	0.260	
CCB001 CCB001	0.529	0.0	0.008	
PB140930BL	0.408	0.0	0.008	
M4759-01	0.506	0.0	0.008	
M4775-02	0.314	0.0	0.007	
M4775-04	0.210	0.0	0.007	
M4775-06	0.539	0.0	0.008	
M4775-08	0.265	0.0	0.007	
M4775-10	0.240	0.0	0.007	
M4775-10DUP	0.329	0.0	0.008	
M4775-10MS	97.094	0.0	0.108	
CCV002 CCV002	246.243	0.0	0.264	
CCB002 CCB002	0.478	0.0	0.008	

N	15
Mean	45.583
SD	87.1497
CV%	191.19

Aquakem v. 7.2AQ1

Results from time period:

Wed Nov 24 13:11:19 2021

Wed Nov 24 13:49:36 2021

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time
S0	A	CNEPA-NE\ P		0.1176	µg/l	11/24/2021 13:11:19
S5.0	A	CNEPA-NE\ P		5.1154	µg/l	11/24/2021 13:11:20
S10.0	A	CNEPA-NE\ P		9.6769	µg/l	11/24/2021 13:11:21
S100.0	A	CNEPA-NE\ P		99.0587	µg/l	11/24/2021 13:11:22
S250.0	A	CNEPA-NE\ P		251.6756	µg/l	11/24/2021 13:11:23
S500.0	A	CNEPA-NE\ P		499.3558	µg/l	11/24/2021 13:11:24
ICV001 ICV001	S	CNEPA-NE\ P		94.0594	µg/l	11/24/2021 13:43:18
ICB001 ICB001	S	CNEPA-NE\ P		0.488	µg/l	11/24/2021 13:43:20
CCV001 CCV001	S	CNEPA-NE\ P		242.0466	µg/l	11/24/2021 13:43:22
CCB001 CCB001	S	CNEPA-NE\ P		0.529	µg/l	11/24/2021 13:43:25
PB140930BL	S	CNEPA-NE\ P		0.4078	µg/l	11/24/2021 13:43:26
M4759-01	S	CNEPA-NE\ P		0.506	µg/l	11/24/2021 13:43:27
M4775-02	S	CNEPA-NE\ P		0.3145	µg/l	11/24/2021 13:43:28
M4775-04	S	CNEPA-NE\ P		0.2097	µg/l	11/24/2021 13:49:29
M4775-06	S	CNEPA-NE\ P		0.5391	µg/l	11/24/2021 13:49:30
M4775-08	S	CNEPA-NE\ P		0.2649	µg/l	11/24/2021 13:49:31
M4775-10	S	CNEPA-NE\ P		0.2404	µg/l	11/24/2021 13:49:32
M4775-10DUP	S	CNEPA-NE\ P		0.3285	µg/l	11/24/2021 13:49:33
M4775-10MS	S	CNEPA-NE\ P		97.094	µg/l	11/24/2021 13:49:34
CCV002 CCV002	S	CNEPA-NE\ P		246.2432	µg/l	11/24/2021 13:49:35
CCB002 CCB002	S	CNEPA-NE\ P		0.4784	µg/l	11/24/2021 13:49:36

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12 Instrument ID : Konelab

11/24/2021 13:13


Test CNEPA-NEW

Accepted 11/24/2021 13:13

Factor 959.1
Bias 0.007

Coeff. of det. 0.999979

Errors

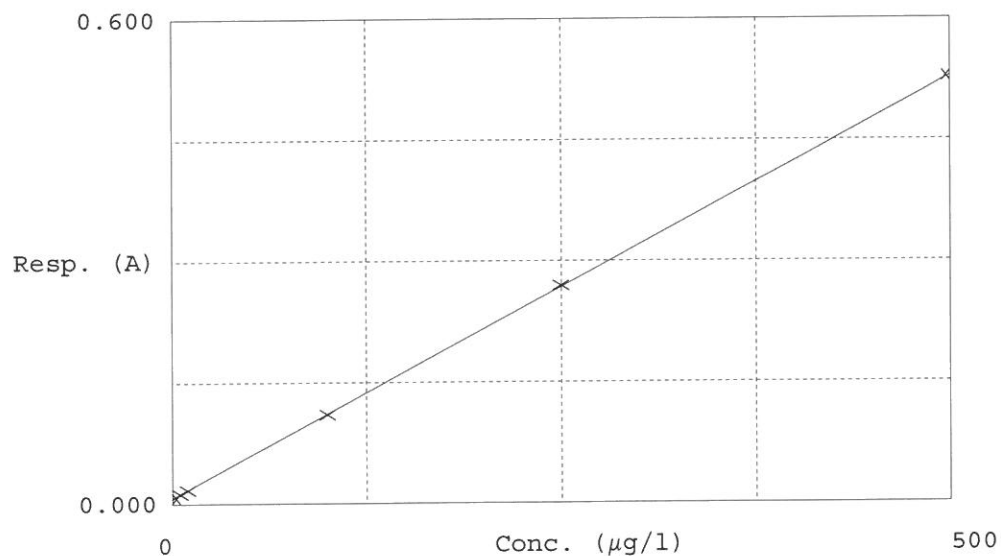

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.007	0.1176	0.0000	—
2	5.0PPBCN	0.013	5.1154	5.0000	2.3
3	10PPBCN	0.017	9.6769	10.0000	-3.2
4	100PPBCN	0.110	99.0587	100.0000	-0.9
5	250PPBCN	0.270	251.6756	250.0000	0.7
6	500PPBCN	0.528	499.3558	500.0000	-0.1

12 11/24/21