

LB117670


7470A

INSTRUMENT ID: CV1

Linear

 μ Abs.:

41297

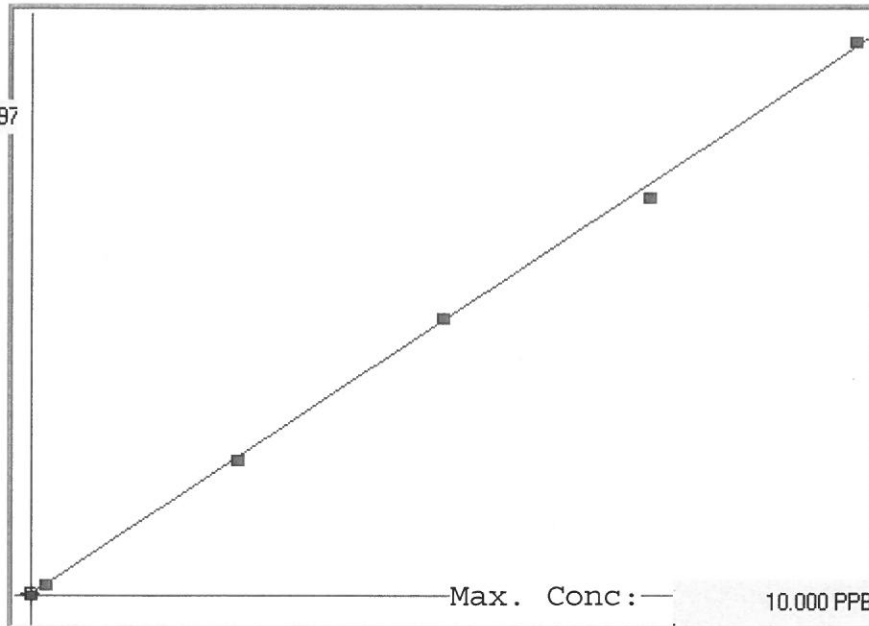

A= 0.0000e+000

B= 2.4516e-004

C= -1.4123e-002

Rho= 0.9996126

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	0.026	0.026	165	0.000	165					1
0.2	0.200	0.202	0.002	880	0.0 %	880					-1
2.5	2.500	2.483	-0.017	10187	0.0 %	10187					2
5.0	5.000	5.085	0.085	20800	0.0 %	20800					-3
7.5	7.500	7.293	-0.207	29805	0.0 %	29805					1
10.0	10.000	10.110	0.110	41297	0.0 %	41297					

LB117670 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 07 Dec 2021 09:50:56

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	165	-	0.0000	7470A	PPB	07 Dec 2021 10:24:17	S	Std
0.2 - 1	50.2	880	-	0.2000	7470A	PPB	07 Dec 2021 10:26:34	S	Std
2.5 - 1	52.5	10187	-	2.5000	7470A	PPB	07 Dec 2021 10:28:51	S	Std
5.0 - 1	55	20800	-	5.0000	7470A	PPB	07 Dec 2021 10:31:08	S	Std
7.5 - 1	57.5	29805	-	7.5000	7470A	PPB	07 Dec 2021 10:33:24	S	Std
10.0 - 1	510	41297	-	10.0000	7470A	PPB	07 Dec 2021 10:35:40	S	Std
ICV98 - 1	ICV98	15247	3.7239	-	7470A	PPB	07 Dec 2021 10:38:26	U	SMPL
ICB98 - 1	ICB98	108	0.0124	-	7470A	PPB	07 Dec 2021 10:40:41	U	SMPL
CCV65 - 1	CCV65	19309	4.7197	-	7470A	PPB	07 Dec 2021 10:42:56	U	SMPL
CCB65 - 1	CCB65	121	0.0155	-	7470A	PPB	07 Dec 2021 10:45:12	U	SMPL
CRA - 1	CRA	898	0.2060	-	7470A	PPB	07 Dec 2021 10:47:26	U	SMPL
HighStd - 1	HighStd	39992	9.7905	-	7470A	PPB	07 Dec 2021 10:49:42	U	SMPL
ChkStd - 1	ChkStd	28031	6.8581	-	7470A	PPB	07 Dec 2021 10:51:57	U	SMPL
PB141200BL - 1	PBW	65	0.0018	-	7470A	PPB	07 Dec 2021 10:56:49	U	SMPL
PB141200BS - 1	LCSW	17066	4.1698	-	7470A	PPB	07 Dec 2021 10:59:05	U	SMPL
M4830-12 - 1	30902:04	433	0.0920	-	7470A	PPB	07 Dec 2021 11:01:22	U	SMPL
M4830-13 - 1	30905:08	518	0.1129	-	7470A	PPB	07 Dec 2021 11:03:38	U	SMPL
M4910-18 - 1	SP-1-4	528	0.1153	-	7470A	PPB	07 Dec 2021 11:05:55	U	SMPL
M4910-20 - 1	SP-1-4	522	0.1139	-	7470A	PPB	07 Dec 2021 11:08:12	U	SMPL
M4920-02 - 1	FDR-20211202-WC-S	526	0.1148	-	7470A	PPB	07 Dec 2021 11:10:27	U	SMPL
CCV66 - 1	CCV66	19401	4.7423	-	7470A	PPB	07 Dec 2021 11:12:42	U	SMPL
CCB66 - 1	CCB66	120	0.0153	-	7470A	PPB	07 Dec 2021 11:14:57	U	SMPL
M4932-02 - 1	DRUM1-2	644	0.1438	-	7470A	PPB	07 Dec 2021 11:17:12	U	SMPL
M4934-01 - 1	XFMR-SHP	506	0.1099	-	7470A	PPB	07 Dec 2021 11:19:28	U	SMPL
M4934-02 - 1	GARAGE-DEBRIS	512	0.1114	-	7470A	PPB	07 Dec 2021 11:21:43	U	SMPL
M4934-03 - 1	17077	187	0.0317	-	7470A	PPB	07 Dec 2021 11:26:36	U	SMPL
M4934-04 - 1	17098	153	0.0234	-	7470A	PPB	07 Dec 2021 11:28:52	U	SMPL
M4936-02 - 1	SLAG-WASTE-CLASS	34	-0.0058	-	7470A	PPB	07 Dec 2021 11:31:08	U	SMPL
M4936-02DUP - 1	SLAG-WASTE-CLASSDUP	-127	-0.0453	-	7470A	PPB	07 Dec 2021 11:33:24	U	SMPL
M4936-02MS - 1	SLAG-WASTE-CLASSMS	13858	3.3834	-	7470A	PPB	07 Dec 2021 11:43:23	U	SMPL
M4936-02MSD - 1	SLAG-WASTE-CLASSMSD	13916	3.3976	-	7470A	PPB	07 Dec 2021 11:45:40	U	SMPL
PB141201BL - 1	PBW	75	0.0043	-	7470A	PPB	07 Dec 2021 11:47:56	U	SMPL
CCV67 - 1	CCV67	19691	4.8134	-	7470A	PPB	07 Dec 2021 11:52:52	U	SMPL
CCB67 - 1	CCB67	70	0.0030	-	7470A	PPB	07 Dec 2021 11:55:07	U	SMPL
M4920-04 - 1	FDR-20211202-WC-W	98	0.0099	-	7470A	PPB	07 Dec 2021 11:59:39	U	SMPL
M4920-04DUP - 1	FDR-20211202-WC-WDUP	116	0.0143	-	7470A	PPB	07 Dec 2021 12:04:27	U	SMPL
M4920-04MS - 1	FDR-20211202-WC-WMS	13498	3.2951	-	7470A	PPB	07 Dec 2021 12:06:43	U	SMPL
M4920-04MSD - 1	FDR-20211202-WC-WMSD	14654	3.5785	-	7470A	PPB	07 Dec 2021 12:08:58	U	SMPL
M4934-05 - 1	17078	421	0.0891	-	7470A	PPB	07 Dec 2021 12:11:14	U	SMPL
M4934-06 - 1	17094	390	0.0815	-	7470A	PPB	07 Dec 2021 12:13:31	U	SMPL
M4934-07 - 1	17097	193	0.0332	-	7470A	PPB	07 Dec 2021 12:15:48	U	SMPL
PB141202BL - 1	PBW	49	-0.0021	-	7470A	PPB	07 Dec 2021 12:18:05	U	SMPL
PB141202BS - 1	LCSW	13144	3.2083	-	7470A	PPB	07 Dec 2021 12:23:05	U	SMPL
CCV68 - 1	CCV68	19322	4.7229	-	7470A	PPB	07 Dec 2021 12:25:19	U	SMPL
CCB68 - 1	CCB68	110	0.0128	-	7470A	PPB	07 Dec 2021 12:27:35	U	SMPL
M4920-03 - 1	FDR-20211202-WC-W	7387	1.7969	-	7470A	PPB	07 Dec 2021 12:29:50	U	SMPL
M4920-03DUP - 1	FDR-20211202-WC-WDUP	6985	1.6983	-	7470A	PPB	07 Dec 2021 12:32:07	U	SMPL
M4920-03MS - 1	FDR-20211202-WC-WMS	21484	5.2530	-	7470A	PPB	07 Dec 2021 12:40:42	U	SMPL
M4920-03MSD - 1	FDR-20211202-WC-WMSD	21708	5.3079	-	7470A	PPB	07 Dec 2021 12:42:57	U	SMPL
PB141200TB - 1	PB141159TB	380	0.0790	-	7470A	PPB	07 Dec 2021 12:45:13	U	SMPL
PB141201TB - 1	PB141161TB	422	0.0893	-	7470A	PPB	07 Dec 2021 12:47:29	U	SMPL
CCV69 - 1	CCV69	20090	4.9112	-	7470A	PPB	07 Dec 2021 12:49:45	U	SMPL
CCB69 - 1	CCB69	99	0.0101	-	7470A	PPB	07 Dec 2021 12:52:02	U	SMPL
M4936-02LX5 - 1		58	0.0001	-	7470A	PPB	07 Dec 2021 12:54:19	U	SMPL
M4936-02A - 1		14510	3.5432	-	7470A	PPB	07 Dec 2021 12:56:34	U	SMPL
M4920-04LX5 - 1		150	0.0227	-	7470A	PPB	07 Dec 2021 12:58:50	U	SMPL
M4920-04A - 1		14604	3.5663	-	7470A	PPB	07 Dec 2021 13:01:06	U	SMPL
M4920-03LX5 - 1		1500	0.3536	-	7470A	PPB	07 Dec 2021 13:03:21	U	SMPL
M4920-03A - 1		23108	5.6511	-	7470A	PPB	07 Dec 2021 13:05:37	U	SMPL
PB141201BS - 1	LCSW	14854	3.6275	-	7470A	PPB	07 Dec 2021 13:15:36	U	SMPL
CCV70 - 1	CCV70	20333	4.9708	-	7470A	PPB	07 Dec 2021 13:17:51	U	SMPL
CCB70 - 1	CCB70	104	0.0114	-	7470A	PPB	07 Dec 2021 13:20:07	U	SMPL