


LB117690

7471B

INSTRUMENT ID: CV1

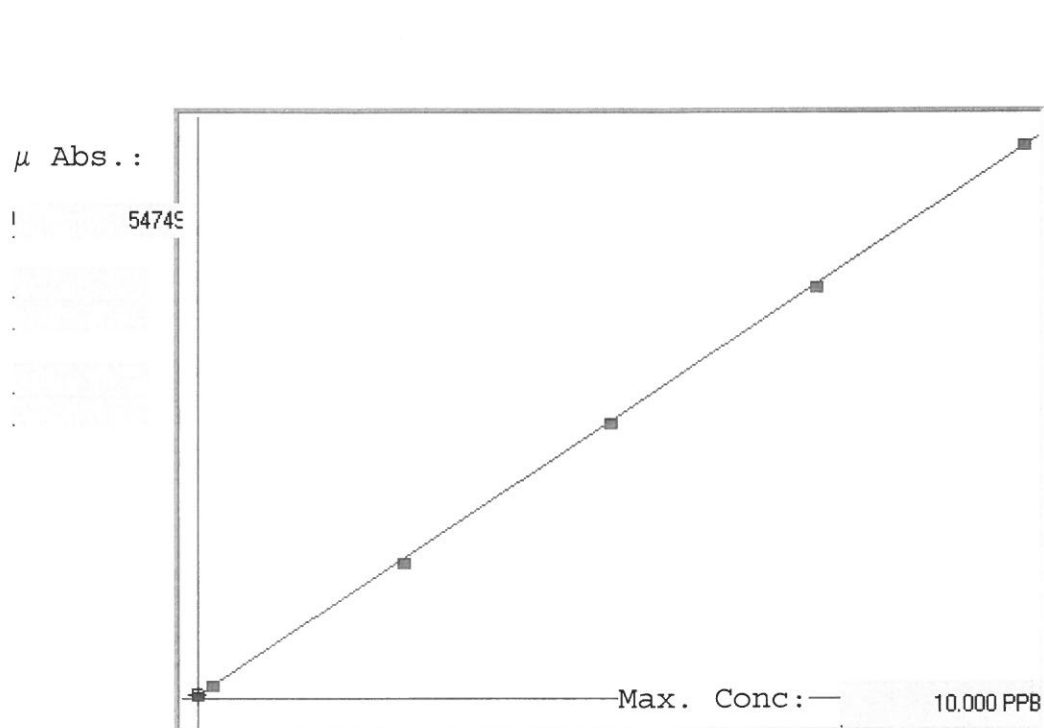

Linear

A= 0.0000e+000

B= 1.8414e-004

C= -4.1418e-002

Rho= 0.9999642

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	0.038	0.038	432	0.000	432					-
0.2	0.200	0.203	0.003	1330	0.0 %	1330					2
2.5	2.500	2.463	-0.037	13601	0.0 %	13601					-1
5.0	5.000	4.992	-0.008	27333	0.0 %	27333					0
7.5	7.500	7.463	-0.037	40756	0.0 %	40756					0
10.0	10.000	10.040	0.040	54749	0.0 %	54749					0

LB117690 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 08 Dec 2021 09:00:43

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	432	-	0.0000	7471B	PPB	08 Dec 2021 09:13:05	S	Std
0.2 - 1	50.2	1330	-	0.2000	7471B	PPB	08 Dec 2021 09:15:22	S	Std
2.5 - 1	52.5	13601	-	2.5000	7471B	PPB	08 Dec 2021 09:17:39	S	Std
5.0 - 1	55	27333	-	5.0000	7471B	PPB	08 Dec 2021 09:19:56	S	Std
7.5 - 1	57.5	40756	-	7.5000	7471B	PPB	08 Dec 2021 09:22:12	S	Std
10.0 - 1	510	54749	-	10.0000	7471B	PPB	08 Dec 2021 09:24:28	S	Std
ICV99 - 1	ICV99	21165	3.8559	-	7471B	PPB	08 Dec 2021 09:27:14	U	SMPL
ICB99 - 1	ICB99	439	0.0394	-	7471B	PPB	08 Dec 2021 09:29:28	U	SMPL
CCV71 - 1	CCV71	26901	4.9122	-	7471B	PPB	08 Dec 2021 09:31:43	U	SMPL
CCB71 - 1	CCB71	436	0.0389	-	7471B	PPB	08 Dec 2021 09:33:58	U	SMPL
CRA - 1	CRA	1307	0.1993	-	7471B	PPB	08 Dec 2021 09:36:14	U	SMPL
HighStd - 1	HighStd	53394	9.7906	-	7471B	PPB	08 Dec 2021 09:38:29	U	SMPL
ChkStd - 1	ChkStd	37170	6.8031	-	7471B	PPB	08 Dec 2021 09:40:45	U	SMPL
PB141234BL - 1	PBS	-11	-0.0434	-	7471B	PPB	08 Dec 2021 09:43:02	U	SMPL
PB141234BS - 1	LCSS	20758	3.7810	-	7471B	PPB	08 Dec 2021 09:45:19	U	SMPL
M4936-01 - 1	SLAG-WASTE-CLASS	15230	2.7631	-	7471B	PPB	08 Dec 2021 09:47:35	U	SMPL
M4944-01 - 1	ETGI-362	44141	8.0868	-	7471B	PPB	08 Dec 2021 09:49:52	U	SMPL
M4945-01 - 1	TP-7-COMP	400	0.0322	-	7471B	PPB	08 Dec 2021 09:52:09	U	SMPL
M4945-01DUP - 1	TP-7-COMPDUP	491	0.0490	-	7471B	PPB	08 Dec 2021 09:54:28	U	SMPL
M4945-01MS - 1	TP-7-COMPMS	19954	3.6329	-	7471B	PPB	08 Dec 2021 09:56:43	U	SMPL
CCV72 - 1	CCV72	26770	4.8880	-	7471B	PPB	08 Dec 2021 09:58:58	U	SMPL
CCB72 - 1	CCB72	410	0.0341	-	7471B	PPB	08 Dec 2021 10:01:13	U	SMPL
M4945-01MSD - 1	TP-7-COMPMSD	20656	3.7622	-	7471B	PPB	08 Dec 2021 10:03:28	U	SMPL
M4946-01 - 1	COMP-5	12162	2.1981	-	7471B	PPB	08 Dec 2021 10:05:43	U	SMPL
M4947-01 - 1	355-994	984	0.1398	-	7471B	PPB	08 Dec 2021 10:07:59	U	SMPL
M4949-01 - 1	VNJ-221	649	0.0781	-	7471B	PPB	08 Dec 2021 10:10:15	U	SMPL
M4955-01 - 1	2022	2360	0.3932	-	7471B	PPB	08 Dec 2021 10:12:30	U	SMPL
M4959-01 - 1	TP-1S	1966	0.3206	-	7471B	PPB	08 Dec 2021 10:14:47	U	SMPL
M4959-04 - 1	TP-1D	660	0.0801	-	7471B	PPB	08 Dec 2021 10:17:03	U	SMPL
M4959-07 - 1	TP-2	2256	0.3740	-	7471B	PPB	08 Dec 2021 10:19:20	U	SMPL
M4959-10 - 1	TP-3S	2343	0.3900	-	7471B	PPB	08 Dec 2021 10:21:37	U	SMPL
M4959-13 - 1	TP-5S	391	0.0306	-	7471B	PPB	08 Dec 2021 10:23:52	U	SMPL
CCV73 - 1	CCV73	27041	4.9379	-	7471B	PPB	08 Dec 2021 10:26:08	U	SMPL
CCB73 - 1	CCB73	433	0.0383	-	7471B	PPB	08 Dec 2021 10:28:23	U	SMPL
M4959-16 - 1	TP-5D	227	0.0004	-	7471B	PPB	08 Dec 2021 10:30:39	U	SMPL
M4959-19 - 1	TP-3D	186	-0.0072	-	7471B	PPB	08 Dec 2021 10:32:54	U	SMPL
M4945-01LX5 - 1		402	0.0326	-	7471B	PPB	08 Dec 2021 10:35:10	U	SMPL
M4945-01A - 1		21433	3.9053	-	7471B	PPB	08 Dec 2021 10:37:25	U	SMPL
CCV74 - 1	CCV74	26930	4.9175	-	7471B	PPB	08 Dec 2021 10:39:42	U	SMPL
CCB74 - 1	CCB74	430	0.0378	-	7471B	PPB	08 Dec 2021 10:41:58	U	SMPL