


LB117698

7470A

INSTRUMENT ID: CV1

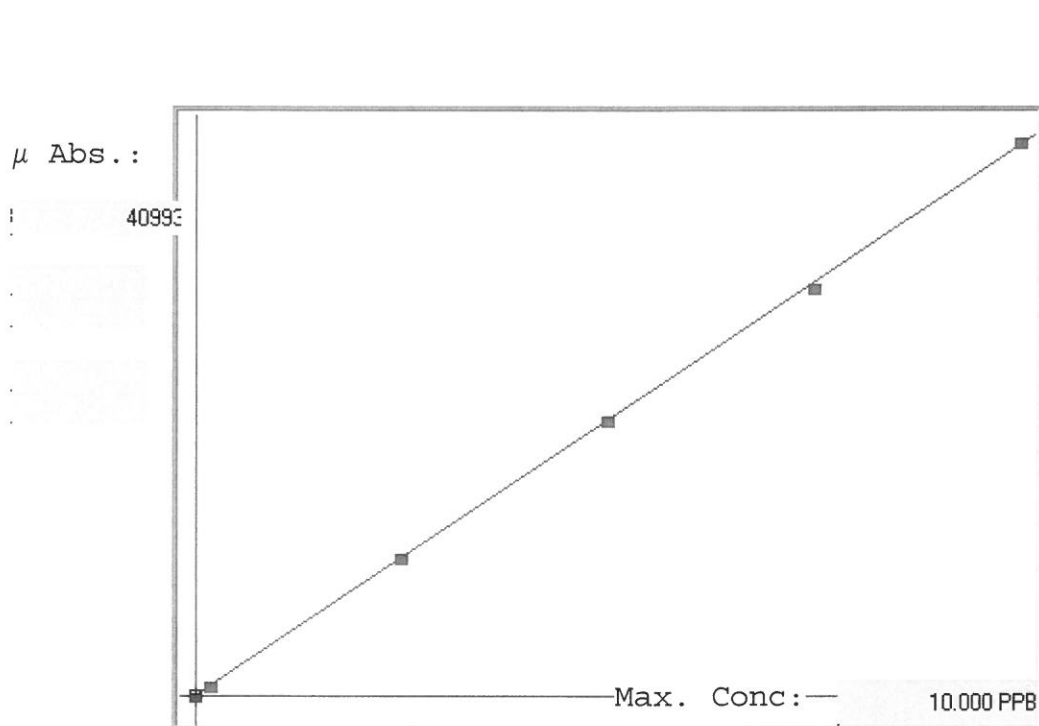

Linear

A= 0.0000e+000

B= 2.4490e-004

C= -3.7351e-003

Rho= 0.9999441

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	90D
0.0	0.000	0.008	0.008	49	0.000	49					1
0.2	0.200	0.179	-0.021	745	0.0 %	745					1
2.5	2.500	2.522	0.022	10314	0.0 %	10314					1
5.0	5.000	5.032	0.032	20563	0.0 %	20563					1
7.5	7.500	7.423	-0.077	30328	0.0 %	30328					1
10.0	10.000	10.035	0.035	40993	0.0 %	40993					0

LB117698 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 08 Dec 2021 14:07:42

Sample ID	Extended ID	μ Abs	Conc.	Std Cond	Method	Units	Date	Type	Type
0.0 - 1	50	49	-	0.0000	7470A	PPB	08 Dec 2021 14:13:41	S	Std
0.2 - 1	50.2	745	-	0.2000	7470A	PPB	08 Dec 2021 14:15:58	S	Std
2.5 - 1	52.5	10314	-	2.5000	7470A	PPB	08 Dec 2021 14:18:15	S	Std
5.0 - 1	55	20563	-	5.0000	7470A	PPB	08 Dec 2021 14:20:32	S	Std
7.5 - 1	57.5	30328	-	7.5000	7470A	PPB	08 Dec 2021 14:22:48	S	Std
10.0 - 1	510	40993	-	10.0000	7470A	PPB	08 Dec 2021 14:25:04	S	Std
ICV02 - 1	ICV02	16495	4.0358	-	7470A	PPB	08 Dec 2021 14:30:12	U	SMPL
ICB02 - 1	ICB02	-11	-0.0064	-	7470A	PPB	08 Dec 2021 14:32:27	U	SMPL
CCV78 - 1	CCV78	19310	4.7252	-	7470A	PPB	08 Dec 2021 14:34:42	U	SMPL
CCB78 - 1	CCB78	-19	-0.0084	-	7470A	PPB	08 Dec 2021 14:36:56	U	SMPL
CRA - 1	CRA	738	0.1770	-	7470A	PPB	08 Dec 2021 14:39:12	U	SMPL
HighStd - 1	HighStd	42038	10.2912	-	7470A	PPB	08 Dec 2021 14:41:27	U	SMPL
ChkStd - 1	ChkStd	28275	6.9207	-	7470A	PPB	08 Dec 2021 14:43:42	U	SMPL
PB141251BL - 1	PBW	-49	-0.0157	-	7470A	PPB	08 Dec 2021 14:45:58	U	SMPL
PB141251BS - 1	LCSW	15745	3.8522	-	7470A	PPB	08 Dec 2021 14:50:46	U	SMPL
M4866-24 - 1	TOTE-SLUDGE	74	0.0144	-	7470A	PPB	08 Dec 2021 14:53:01	U	SMPL
M4945-03 - 1	TP-7-COMP	10	-0.0013	-	7470A	PPB	08 Dec 2021 14:55:18	U	SMPL
M4946-02 - 1	COMP-5	30	0.0036	-	7470A	PPB	08 Dec 2021 14:57:34	U	SMPL
M4947-02 - 1	355-994	46	0.0075	-	7470A	PPB	08 Dec 2021 14:59:51	U	SMPL
M4958-01 - 1	D-01	52	0.0090	-	7470A	PPB	08 Dec 2021 15:02:07	U	SMPL
CCV79 - 1	CCV79	20376	4.9863	-	7470A	PPB	08 Dec 2021 15:04:22	U	SMPL
CCB79 - 1	CCB79	-17	-0.0079	-	7470A	PPB	08 Dec 2021 15:06:37	U	SMPL
M4959-02 - 1	TP-1S	55	0.0097	-	7470A	PPB	08 Dec 2021 15:08:53	U	SMPL
M4959-05 - 1	TP-1D	69	0.0132	-	7470A	PPB	08 Dec 2021 15:11:08	U	SMPL
M4959-08 - 1	TP-2	36	0.0051	-	7470A	PPB	08 Dec 2021 15:13:23	U	SMPL
M4959-11 - 1	TP-3S	33	0.0043	-	7470A	PPB	08 Dec 2021 15:15:39	U	SMPL
M4959-14 - 1	TP-5S	36	0.0051	-	7470A	PPB	08 Dec 2021 15:17:55	U	SMPL
M4959-17 - 1	TP-5D	41	0.0063	-	7470A	PPB	08 Dec 2021 15:20:11	U	SMPL
M4959-20 - 1	TP-3D	48	0.0080	-	7470A	PPB	08 Dec 2021 15:22:28	U	SMPL
M4965-03 - 1	RED-CONCRETE-COMP-EXTERIOR	39	0.0058	-	7470A	PPB	08 Dec 2021 15:24:44	U	SMPL
M4965-09 - 1	WHITE-CONCRETE-COMP-EXTERIOR	37	0.0053	-	7470A	PPB	08 Dec 2021 15:27:01	U	SMPL
M4965-15 - 1	BLUE-CONCRETE-COMP	36	0.0051	-	7470A	PPB	08 Dec 2021 15:29:17	U	SMPL
CCV80 - 1	CCV80	21074	5.1572	-	7470A	PPB	08 Dec 2021 15:31:33	U	SMPL
CCB80 - 1	CCB80	-25	-0.0099	-	7470A	PPB	08 Dec 2021 15:33:48	U	SMPL
M4965-21 - 1	RED-WALL-CONCRETE-COMP	30	0.0036	-	7470A	PPB	08 Dec 2021 15:36:04	U	SMPL
M4965-27 - 1	WHITE-BROWN-CONCRETE-COMP	28	0.0031	-	7470A	PPB	08 Dec 2021 15:38:19	U	SMPL
M4965-32 - 1	FLOORS-COMP	18	0.0007	-	7470A	PPB	08 Dec 2021 15:40:35	U	SMPL
M4965-32DUP - 1	FLOORS-COMPDUP	20	0.0012	-	7470A	PPB	08 Dec 2021 15:42:51	U	SMPL
M4965-32MS - 1	FLOORS-COMPMS	15723	3.8468	-	7470A	PPB	08 Dec 2021 15:47:40	U	SMPL
M4965-32MSD - 1	FLOORS-COMPMSD	15764	3.8568	-	7470A	PPB	08 Dec 2021 15:49:56	U	SMPL
PB141251TB - 1	PB141230TB	-18	-0.0081	-	7470A	PPB	08 Dec 2021 15:52:13	U	SMPL
M4965-32LX5 - 1		32	0.0041	-	7470A	PPB	08 Dec 2021 15:54:30	U	SMPL
M4965-32A - 1		16525	4.0432	-	7470A	PPB	08 Dec 2021 15:56:46	U	SMPL
CCV81 - 1	CCV81	19447	4.7588	-	7470A	PPB	08 Dec 2021 15:59:02	U	SMPL
CCB81 - 1	CCB81	-26	-0.0101	-	7470A	PPB	08 Dec 2021 16:01:18	U	SMPL