

LB117768

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : il Instrument ID : Konelab

12/13/2021 14:04

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	95.465	0.0	0.079	
ICB1	0.575	0.0	0.001	
CCV1	241.180	0.0	0.199	
CCB1	0.642	0.0	0.001	
PB141342BL	0.543	0.0	0.001	
PB141342BS	94.534	0.0	0.078	
MIDPB141342	241.662	0.0	0.200	
M5061-01	0.293	0.0	0.001	
M5061-0DUP	0.635	0.0	0.001	
M5061-01MS	27.556	0.0	0.023	
M5061-01MSD	27.667	0.0	0.023	
CCV2	247.412	0.0	0.204	
CCB2	0.550	0.0	0.001	

N	13
Mean	75.286
SD	101.5197
CV%	134.85

Aquakem v. 7.2AQ1

Results from time period:

Mon Dec 13 13:51:32 2021

Mon Dec 13 13:57:50 2021

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time
0.OPPBCN	A	Total CN	P	0.5397	µg/l	12/13/2021 11:45:03
5.OPPBCN	A	Total CN	P	4.496	µg/l	12/13/2021 11:45:04
10PPBCN	A	Total CN	P	9.1584	µg/l	12/13/2021 11:45:05
50PPBCN	A	Total CN	P	48.4799	µg/l	12/13/2021 11:45:06
100PPBCN	A	Total CN	P	99.8412	µg/l	12/13/2021 11:45:07
250PPBCN	A	Total CN	P	254.5582	µg/l	12/13/2021 11:45:08
500PPBCN	A	Total CN	P	497.9265	µg/l	12/13/2021 11:45:09
ICV1	S	Total CN	P	95.4648	µg/l	12/13/2021 13:51:33
ICB1	S	Total CN	P	0.5749	µg/l	12/13/2021 13:51:34
CCV1	S	Total CN	P	241.1805	µg/l	12/13/2021 13:51:37
CCB1	S	Total CN	P	0.6422	µg/l	12/13/2021 13:51:39
PB141342BL	S	Total CN	P	0.5426	µg/l	12/13/2021 13:51:40
PB141342BS	S	Total CN	P	94.5339	µg/l	12/13/2021 13:51:41
MIDPB141342	S	Total CN	P	241.6618	µg/l	12/13/2021 13:51:42
M5061-01	S	Total CN	P	0.2926	µg/l	12/13/2021 13:57:43
M5061-0DUP	S	Total CN	P	0.6352	µg/l	12/13/2021 13:57:44
M5061-01MS	S	Total CN	P	27.5556	µg/l	12/13/2021 13:57:47
M5061-01MSD	S	Total CN	P	27.6668	µg/l	12/13/2021 13:57:48
CCV2	S	Total CN	P	247.412	µg/l	12/13/2021 13:57:49
CCB2	S	Total CN	P	0.55	µg/l	12/13/2021 13:57:50

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12 Instrument ID : Konelab

12/13/2021 11:55

Test Total CN


Accepted 12/13/2021 11:55

Factor 1212

Bias 0

Coeff. of det. 0.999861

Errors

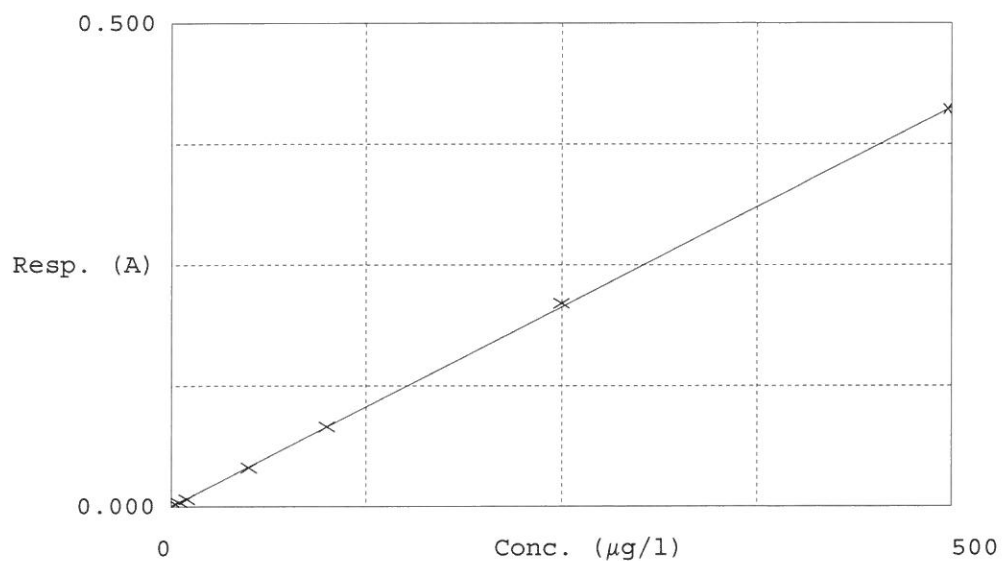

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.001	0.5397	0.0000	-
2	5.0PPBCN	0.004	4.4960	5.0000	-10.1
3	10PPBCN	0.008	9.1584	10.0000	-8.4
4	50PPBCN	0.040	48.4799	50.0000	-3.0
5	100PPBCN	0.083	99.8412	100.0000	-0.2
6	250PPBCN	0.210	254.5582	250.0000	1.8
7	500PPBCN	0.411	497.9265	500.0000	-0.4

12 12/13/21