


LB 117870

7470A

INSTRUMENT ID: CV1

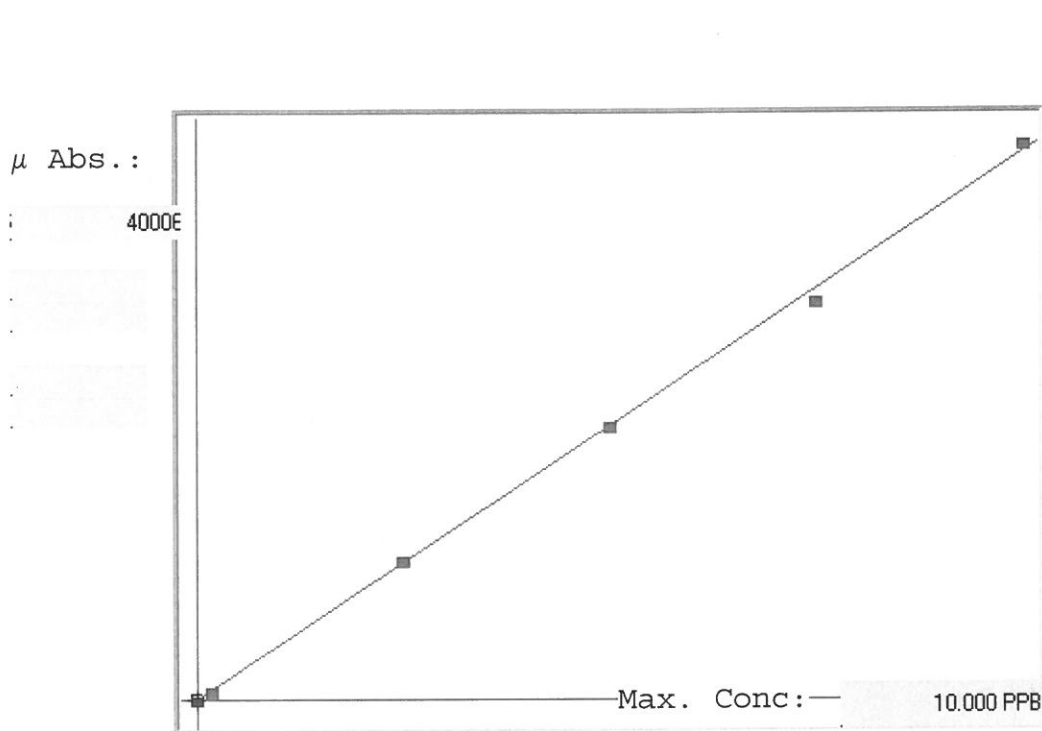

A= 0.0000e+000

B= 2.5307e-004

C= 1.5368e-002

Rho= 0.9995683

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	0.039	0.039	92	0.000	92					-12
0.2	0.200	0.176	-0.024	635	0.0 %	635					3
2.5	2.500	2.565	0.065	10074	0.0 %	10074					0
5.0	5.000	4.992	-0.008	19666	0.0 %	19666					-3
7.5	7.500	7.289	-0.211	28740	0.0 %	28740					1
10.0	10.000	10.140	0.140	40006	0.0 %	40006					

LB117870 INSTRUMENT ID : CV1

Method: 7470A		Operator: Admin		Date of Analysis: 18 Dec 2021 11:18:59					
Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	92	-	0.00007470A	PPB		18 Dec 2021 11:27:38	S	Std
0.2 - 1	50.2	635	-	0.20007470A	PPB		18 Dec 2021 11:29:55	S	Std
2.5 - 1	52.5	10074	-	2.50007470A	PPB		18 Dec 2021 11:32:13	S	Std
5.0 - 1	55	19666	-	5.00007470A	PPB		18 Dec 2021 11:34:30	S	Std
7.5 - 1	57.5	28740	-	7.50007470A	PPB		18 Dec 2021 11:36:46	S	Std
10.0 - 1	58	40006	-	10.00007470A	PPB		18 Dec 2021 11:39:02	S	Std
ICV17 - 1	ICV17	14620	3.7152	-7470A	PPB		18 Dec 2021 11:41:43	U	SMPL
ICB17 - 1	ICB17	-13	0.0121	-7470A	PPB		18 Dec 2021 11:43:57	U	SMPL
CCV50 - 1	CCV50	19328	4.9067	-7470A	PPB		18 Dec 2021 11:46:12	U	SMPL
CCB50 - 1	CCB50	-29	0.0080	-7470A	PPB		18 Dec 2021 11:48:27	U	SMPL
CRA - 1	CRA	614	0.1708	-7470A	PPB		18 Dec 2021 11:50:42	U	SMPL
HighStd - 1	HighStd	39887	10.1096	-7470A	PPB		18 Dec 2021 11:52:57	U	SMPL
ChkStd - 1	ChkStd	27648	7.0122	-7470A	PPB		18 Dec 2021 11:55:12	U	SMPL
PB141525BL - 1	PBW	-45	0.0040	-7470A	PPB		18 Dec 2021 11:57:29	U	SMPL
PB141525BS - 1	LCSW	15244	3.8732	-7470A	PPB		18 Dec 2021 12:02:16	U	SMPL
M5124-02 - 1	F2337-STOPJOINT-TP	-6	0.0138	-7470A	PPB		18 Dec 2021 12:04:32	U	SMPL
M5129-01 - 1	48-CI-1	14	0.0189	-7470A	PPB		18 Dec 2021 12:06:49	U	SMPL
M5129-03 - 1	48-CI-2	52	0.0285	-7470A	PPB		18 Dec 2021 12:09:06	U	SMPL
M5129-03DUP - 1	48-CI-2DUP	57	0.0298	-7470A	PPB		18 Dec 2021 12:11:23	U	SMPL
M5129-03MS - 1	48-CI-2MS	15728	3.9956	-7470A	PPB		18 Dec 2021 12:16:08	U	SMPL
CCV51 - 1	CCV51	19513	4.9535	-7470A	PPB		18 Dec 2021 12:18:23	U	SMPL
CCB51 - 1	CCB51	-25	0.0090	-7470A	PPB		18 Dec 2021 12:20:38	U	SMPL
M5129-03MSD - 1	48-CI-2MSD	17203	4.3689	-7470A	PPB		18 Dec 2021 12:22:53	U	SMPL
PB141526BL - 1	PBW	-30	0.0078	-7470A	PPB		18 Dec 2021 12:25:08	U	SMPL
PB141526BS - 1	LCSW	16257	4.1295	-7470A	PPB		18 Dec 2021 12:30:04	U	SMPL
M5083-22 - 1	BB1	-12	0.0123	-7470A	PPB		18 Dec 2021 12:32:20	U	SMPL
M5083-23 - 1	BB2	22	0.0209	-7470A	PPB		18 Dec 2021 12:34:35	U	SMPL
M5083-24 - 1	BB3	20	0.0204	-7470A	PPB		18 Dec 2021 12:36:51	U	SMPL
M5083-25 - 1	BB4	26	0.0219	-7470A	PPB		18 Dec 2021 12:39:08	U	SMPL
M5083-26 - 1	BB5	19	0.0202	-7470A	PPB		18 Dec 2021 12:41:25	U	SMPL
M5083-27 - 1	BB6	39	0.0252	-7470A	PPB		18 Dec 2021 12:43:42	U	SMPL
M5086-03 - 1	14ST-SP-121421	21	0.0207	-7470A	PPB		18 Dec 2021 12:45:58	U	SMPL
CCV52 - 1	CCV52	19626	4.9821	-7470A	PPB		18 Dec 2021 12:48:13	U	SMPL
CCB52 - 1	CCB52	-17	0.0111	-7470A	PPB		18 Dec 2021 12:50:29	U	SMPL
M5089-03 - 1	MS-1	13	0.0187	-7470A	PPB		18 Dec 2021 12:52:44	U	SMPL
M5089-07 - 1	MS-2	58	0.0300	-7470A	PPB		18 Dec 2021 12:55:00	U	SMPL
M5089-11 - 1	MS-3	25	0.0217	-7470A	PPB		18 Dec 2021 12:57:16	U	SMPL
M5089-15 - 1	MS-4	21	0.0207	-7470A	PPB		18 Dec 2021 12:59:31	U	SMPL
M5089-15DUP - 1	MS-4DUP	41	0.0257	-7470A	PPB		18 Dec 2021 13:01:47	U	SMPL
M5089-15MS - 1	MS-4MS	15556	3.9521	-7470A	PPB		18 Dec 2021 13:04:04	U	SMPL
M5089-15MSD - 1	MS-4MSD	15394	3.9111	-7470A	PPB		18 Dec 2021 13:06:20	U	SMPL
PB141525TB - 1	PB141494TB	-27	0.0085	-7470A	PPB		18 Dec 2021 13:08:36	U	SMPL
PB141526TB - 1	PB141432TB	23	0.0212	-7470A	PPB		18 Dec 2021 13:10:53	U	SMPL
CCV53 - 1	CCV53	19852	5.0393	-7470A	PPB		18 Dec 2021 13:13:10	U	SMPL
CCB53 - 1	CCB53	-34	0.0068	-7470A	PPB		18 Dec 2021 13:15:26	U	SMPL
M5129-03LX5 - 1		36	0.0245	-7470A	PPB		18 Dec 2021 13:17:42	U	SMPL
M5129-03A - 1		16018	4.0690	-7470A	PPB		18 Dec 2021 13:19:57	U	SMPL
M5089-15LX5 - 1		-43	0.0045	-7470A	PPB		18 Dec 2021 13:22:13	U	SMPL
M5089-15A - 1		16254	4.1288	-7470A	PPB		18 Dec 2021 13:24:28	U	SMPL
CCV54 - 1	CCV54	19465	4.9414	-7470A	PPB		18 Dec 2021 13:26:44	U	SMPL
CCB54 - 1	CCB54	-25	0.0090	-7470A	PPB		18 Dec 2021 13:29:01	U	SMPL