


7470A

LB117939

INSTRUMENT ID: CV1

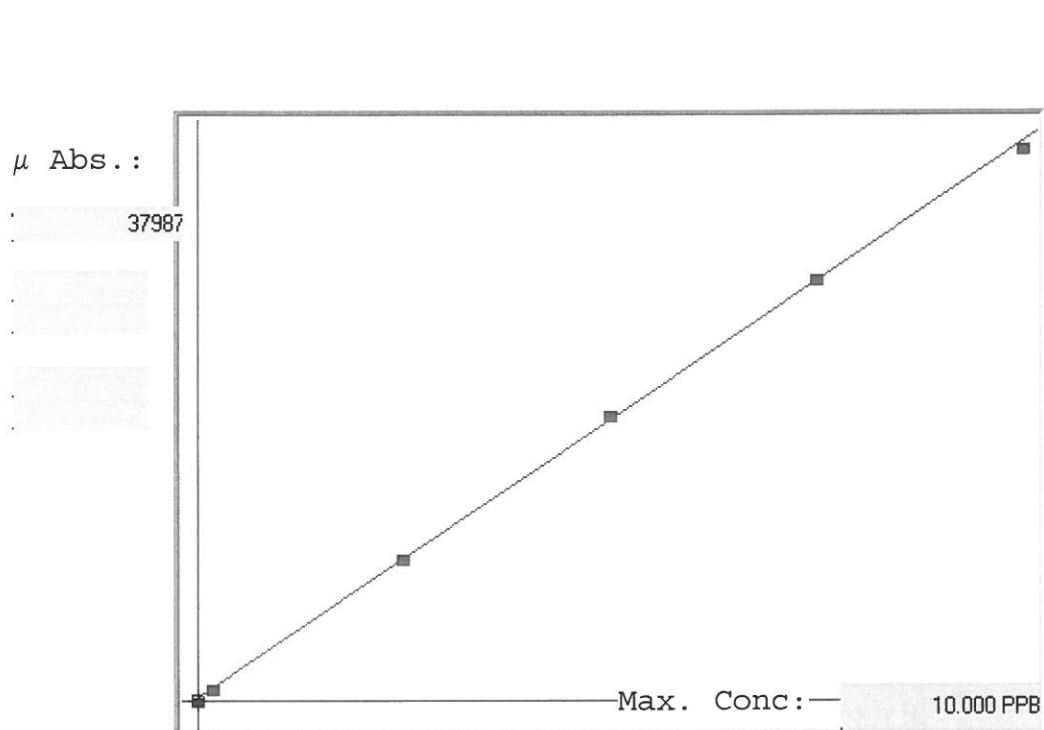

Linear

A= 0.0000e+000

B= 2.6188e-004

C= -4.2549e-002

Rho= 0.9998551

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	70D
0.0	0.000	-0.044	-0.044	-4	0.000	-4					-12
0.2	0.200	0.177	-0.023	838	0.0 %	838					0
2.5	2.500	2.509	0.009	9744	0.0 %	9744					2
5.0	5.000	5.095	0.095	19617	0.0 %	19617					1
7.5	7.500	7.557	0.057	29019	0.0 %	29019					1
10.0	10.000	9.906	-0.094	37987	0.0 %	37987					-1

LB117939 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 23 Dec 2021 09:25:22

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	-4	-	0.0000	7470A	PPB	23 Dec 2021 09:45:39	S	Std
0.2 - 1	50.2	838	-	0.2000	7470A	PPB	23 Dec 2021 09:47:55	S	Std
2.5 - 1	52.5	9744	-	2.5000	7470A	PPB	23 Dec 2021 09:50:12	S	Std
5.0 - 1	55	19617	-	5.0000	7470A	PPB	23 Dec 2021 09:52:29	S	Std
7.5 - 1	57.5	29019	-	7.5000	7470A	PPB	23 Dec 2021 09:54:46	S	Std
10.0 - 1	510	37987	-	10.0000	7470A	PPB	23 Dec 2021 09:57:01	S	Std
ICV23 - 1	ICV23	15825	4.1018	-	7470A	PPB	23 Dec 2021 09:59:45	U	SMPL
ICB23 - 1	ICB23	-18	-0.0473	-	7470A	PPB	23 Dec 2021 10:02:00	U	SMPL
CCV87 - 1	CCV87	18782	4.8761	-	7470A	PPB	23 Dec 2021 10:04:14	U	SMPL
CCB87 - 1	CCB87	-23	-0.0486	-	7470A	PPB	23 Dec 2021 10:06:29	U	SMPL
CRA - 1	CRA	865	0.1840	-	7470A	PPB	23 Dec 2021 10:08:44	U	SMPL
HighStd - 1	HighStd	38218	9.9661	-	7470A	PPB	23 Dec 2021 10:10:59	U	SMPL
ChkStd - 1	ChkStd	27649	7.1983	-	7470A	PPB	23 Dec 2021 10:13:14	U	SMPL
PB141644BL - 1	PBW	-69	-0.0606	-	7470A	PPB	23 Dec 2021 10:15:31	U	SMPL
PB141644BS - 1	LCSW	15860	4.1109	-	7470A	PPB	23 Dec 2021 10:28:54	U	SMPL
M5197-01 - 1	AUD-1230	220	0.0151	-	7470A	PPB	23 Dec 2021 10:31:10	U	SMPL
M5197-01DUP - 1	AUD-1230DUP	269	0.0279	-	7470A	PPB	23 Dec 2021 10:33:27	U	SMPL
M5197-01MS - 1	AUD-1230MS	15794	4.0936	-	7470A	PPB	23 Dec 2021 10:35:43	U	SMPL
M5197-01MSD - 1	AUD-1230MSD	15523	4.0227	-	7470A	PPB	23 Dec 2021 10:38:00	U	SMPL
M5197-03 - 1	AUD-1231	244	0.0214	-	7470A	PPB	23 Dec 2021 10:40:15	U	SMPL
CCV88 - 1	CCV88	19415	5.0419	-	7470A	PPB	23 Dec 2021 10:42:31	U	SMPL
CCB88 - 1	CCB88	-58	-0.0577	-	7470A	PPB	23 Dec 2021 10:44:46	U	SMPL
M5197-05 - 1	AUD-1233-1234	441	0.0729	-	7470A	PPB	23 Dec 2021 10:47:02	U	SMPL
PB141645BL - 1	PBW	1	-0.0423	-	7470A	PPB	23 Dec 2021 10:49:17	U	SMPL
PB141645BS - 1	LCSW	15740	4.0795	-	7470A	PPB	23 Dec 2021 10:51:33	U	SMPL
M5182-03 - 1	EQUIPMENT-BLANK	380	0.0570	-	7470A	PPB	23 Dec 2021 10:53:49	U	SMPL
M5182-03DUP - 1	EQUIPMENT-BLANKDUP	431	0.0703	-	7470A	PPB	23 Dec 2021 10:58:42	U	SMPL
M5182-03MS - 1	EQUIPMENT-BLANKMS	15613	4.0462	-	7470A	PPB	23 Dec 2021 11:00:58	U	SMPL
M5182-03MSD - 1	EQUIPMENT-BLANKMSD	16213	4.2034	-	7470A	PPB	23 Dec 2021 11:03:15	U	SMPL
PB141644TB - 1	PB141635TB	383	0.0578	-	7470A	PPB	23 Dec 2021 11:05:32	U	SMPL
CCV89 - 1	CCV89	19500	5.0642	-	7470A	PPB	23 Dec 2021 11:07:49	U	SMPL
CCB89 - 1	CCB89	-41	-0.0533	-	7470A	PPB	23 Dec 2021 11:10:05	U	SMPL
M5197-01LX5 - 1		37	-0.0329	-	7470A	PPB	23 Dec 2021 11:12:20	U	SMPL
M5197-01A - 1		18187	4.7203	-	7470A	PPB	23 Dec 2021 11:14:36	U	SMPL
M5182-03LX5 - 1		23	-0.0365	-	7470A	PPB	23 Dec 2021 11:16:52	U	SMPL
M5182-03A - 1		18149	4.7104	-	7470A	PPB	23 Dec 2021 11:19:07	U	SMPL
CCV90 - 1	CCV90	19003	4.9340	-	7470A	PPB	23 Dec 2021 11:21:23	U	SMPL
CCB90 - 1	CCB90	-39	-0.0528	-	7470A	PPB	23 Dec 2021 11:23:39	U	SMPL