

Clear table

Instrument ID: IC-2 Analyst : IZ Method: 300.0 / 9056A

ident	concentra tion F-	concentratio n CL-	concentratio on NO2	concentratio on BR-	concentratio on NO3	concentratio on HPO4	concentratio on SO4	file name	date time	Initial wt/ Final Vol	Analyst
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2021-12-09_	12/9/21 10:57		IZ/AP
STD2	0.4870	0.7130	0.7080	2.3930	0.6040	0.8310	3.7470	2021-12-09_	12/9/21 11:25		IZ/AP
STD3	0.8250	1.2360	1.2260	4.1070	1.0350	2.1100	6.1950	2021-12-09_	12/9/21 11:54		IZ/AP
STD4	1.0510	1.4950	1.4920	4.9660	1.2470	2.6630	7.4650	2021-12-09_	12/9/21 12:23		IZ/AP
STD5	1.8730	2.8860	2.9010	9.6190	2.3860	4.9980	14.2340	2021-12-09_	12/9/21 12:51		IZ/AP
STD6	3.7810	5.7700	5.7910	19.2710	4.8030	9.7350	28.7290	2021-12-09_	12/9/21 13:20		IZ/AP
STD7	5.1830	7.6990	7.6820	25.6430	6.4240	12.6630	38.6310	2021-12-09_	12/9/21 13:49		IZ/AP
ICV	1.8470	2.8370	2.8540	9.4540	2.3550	4.8790	14.0120	2021-12-09_	12/9/21 14:25		IZ/AP
ICB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2021-12-09_	12/9/21 14:55		IZ/AP
CCV	2.0620	2.9670	2.9610	9.9450	2.4340	4.6470	14.5970	2021-12-23_	12/23/21 8:54		IZ/AP
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2021-12-23_	12/23/21 9:23		IZ/AP
LB117940BLW	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2021-12-23_	12/23/21 9:53		IZ/AP
LB117940BSW	2.0210	2.9670	2.9860	9.9690	2.4430	4.8330	14.6470	2021-12-23_	12/23/21 10:22		IZ/AP
M5205-01X100	0.0000	13.0960	0.0000	0.0000	0.0000	0.0000	0.0000	2021-12-23_	12/23/21 10:53		IZ/AP
M5205-01MSX100	0.0000	12.3860	0.2440	0.0000	0.2320	-0.3150	0.0000	2021-12-23_	12/23/21 11:22		IZ/AP
M5205-01MSDX100	0.0000	12.5310	0.2410	0.8770	0.2310	-0.3330	0.0000	2021-12-23_	12/23/21 11:51		IZ/AP
M5205-01DLX300	0.0000	4.0910	0.0000	0.0000	0.0000	0.0000	0.0000	2021-12-23_	12/23/21 12:20		IZ/AP
CCV	2.1520	2.9580	2.9810	9.9310	2.4420	5.4890	14.6190	2021-12-23_	12/23/21 12:50		IZ/AP
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2021-12-23_	12/23/21 13:19		IZ/AP

Clear table

Instrument ID: IC-2 Analyst : IZ Method: 300 / 9056A


ident	concentra tion F-	concentratio n CL-	concentratio on NO2	concentratio on BR-	concentratio on NO3	concentratio on HPO4	concentratio on SO4	file name	date time	Initial wt/ Final Vol	Analyst
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2021-12-09_	12/9/21 10:57		IZ/AP
STD2	0.4870	0.7130	0.7080	2.3930	0.6040	0.8310	3.7470	2021-12-09_	12/9/21 11:25		IZ/AP
STD3	0.8250	1.2360	1.2260	4.1070	1.0350	2.1100	6.1950	2021-12-09_	12/9/21 11:54		IZ/AP
STD4	1.0510	1.4950	1.4920	4.9660	1.2470	2.6630	7.4650	2021-12-09_	12/9/21 12:23		IZ/AP
STD5	1.8730	2.8860	2.9010	9.6190	2.3860	4.9980	14.2340	2021-12-09_	12/9/21 12:51		IZ/AP
STD6	3.7810	5.7700	5.7910	19.2710	4.8030	9.7350	28.7290	2021-12-09_	12/9/21 13:20		IZ/AP
STD7	5.1830	7.6990	7.6820	25.6430	6.4240	12.6630	38.6310	2021-12-09_	12/9/21 13:49		IZ/AP

ident	True Value	True Value	True Value	True Value	True Value	True Value	True Value
	CL-	NO2	BR-	NO3	HPO4	SO4	
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	
STD2	0.4000	0.6000	2.0000	0.5000	1.0000	3.0000	
STD3	0.8000	1.2000	4.0000	1.0000	2.0000	6.0000	
STD4	1.0000	1.5000	5.0000	1.2500	2.5000	7.5000	
STD5	2.0000	3.0000	10.0000	2.5000	5.0000	15.0000	
STD6	4.0000	6.0000	20.0000	5.0000	10.0000	30.0000	
STD7	5.0000	7.5000	25.0000	6.2500	12.5000	37.5000	

ident	Relative Error F-	Relative Error CL-	Relative Error NO2	Relative Error BR-	Relative Error NO3	Relative Error HPO4	Relative Error SO4
STD1		18.8333	18.0000	19.6500	20.8000	-16.9000	24.9000
STD2	21.7500	3.0000	2.1667	2.6750	3.5000	5.5000	3.2500
STD3	3.1250	-0.3333	-0.5333	-0.6800	-0.2400	6.5200	-0.4667
STD4	5.1000	-3.8000	-3.3000	-3.8100	-4.5600	-0.0400	-5.1067
STD5	-6.3500	-3.8333	-3.4833	-3.6450	-3.9400	-2.6500	-4.2367
STD6	-5.4750	2.6533	2.4267	2.5720	2.7840	1.3040	3.0160
STD7	3.6600						

CALIBRATION OF COMPONENT F-

Method: AnionsIC2-120921.mtw
 Equation: $Q = 0.061191 \cdot A + 4.51587$
 RSD: 7.496 %
 Correlation coefficient: 0.996932

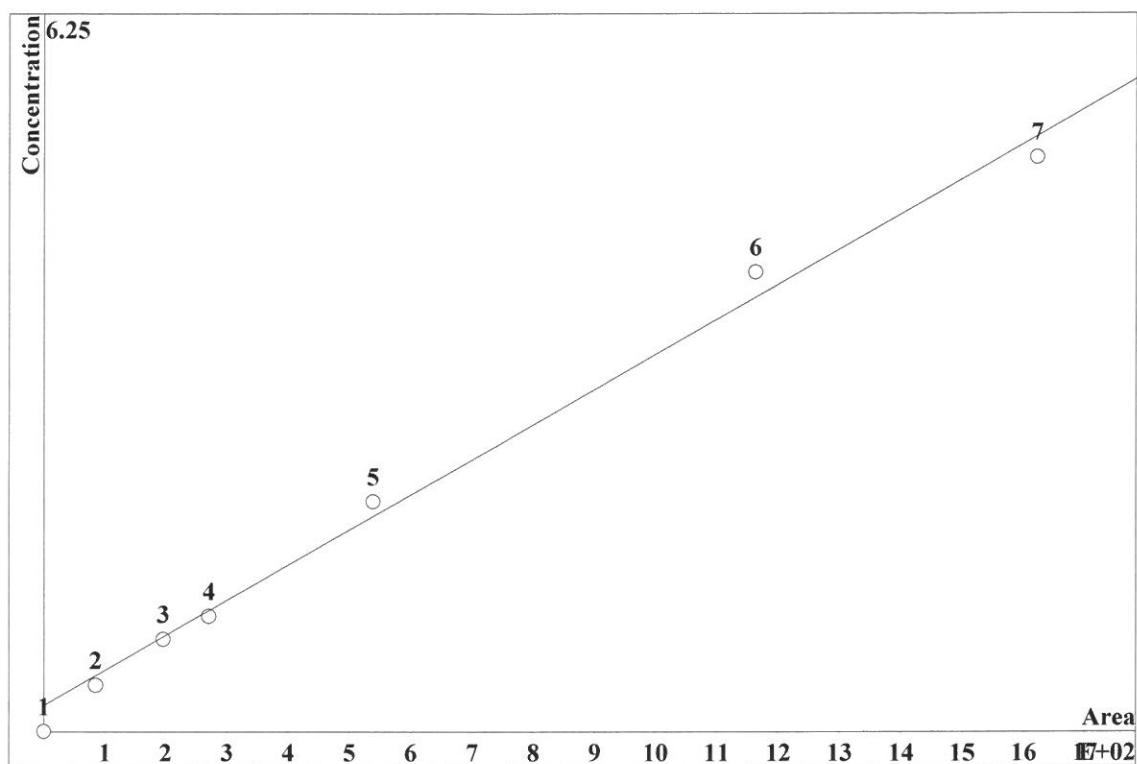

K3 = 0 K2 = 0 K1 = 0.061191 K0 = 4.51587

Base: Area

Ref.channel: ch1

ISTD:


Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	4.365	85.32	0.4	20	5.681		
3	10.27	195.9	0.8	20	5.681		
4	15.18	269.9	1	20	5.681		
5	29.78	538.2	2	20	5.681		
6	69.12	1162	4	20	5.681		
7	103.4	1620	5	20	5.681		

CALIBRATION OF COMPONENT CL-

Method: AnionsIC2-120921.mtw
 Equation: $Q = 0.105567 \cdot A + 4.21377$
 RSD: 5.240 %
 Correlation coefficient: 0.998502

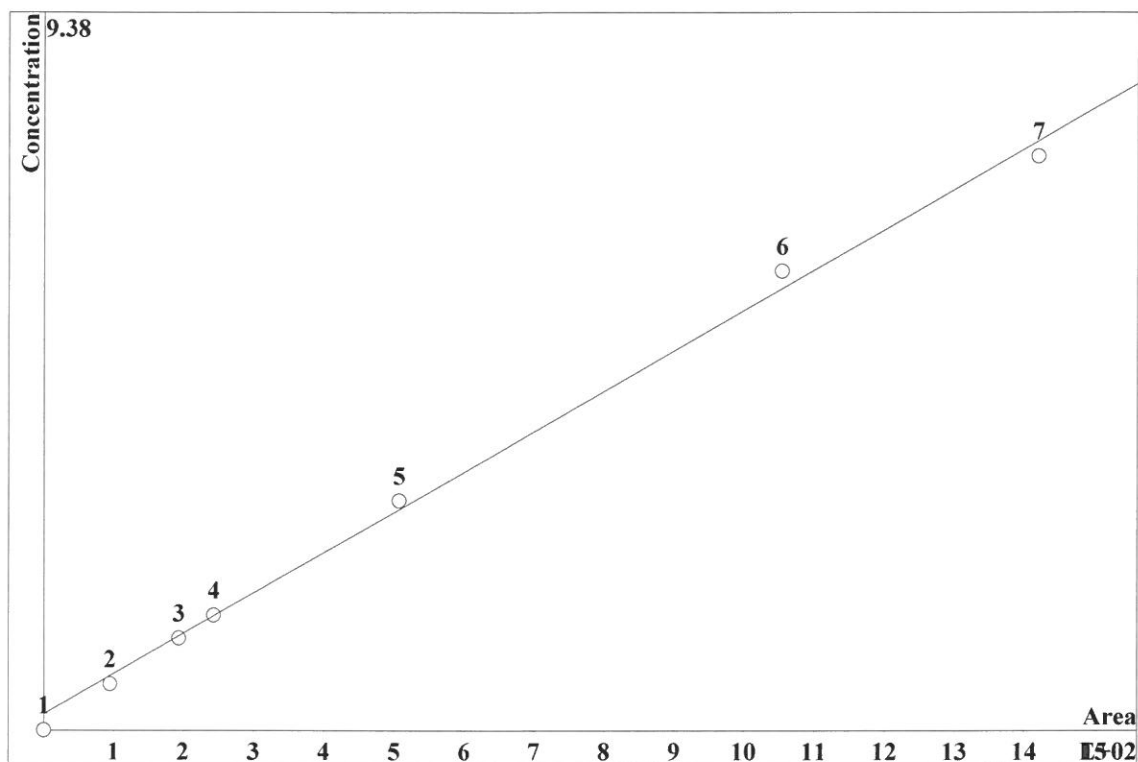

K3 = 0 K2 = 0 K1 = 0.105567 K0 = 4.21377

Base: Area

Ref.channel: chl

ISTD:


Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	7.093	95.25	0.6	20	8.597		
3	14.5	194.2	1.2	20	8.597		
4	18.21	243.3	1.5	20	8.597		
5	38.42	506.9	3	20	8.597		
6	81.59	1053	6	20	8.597		
7	111.1	1419	7.5	20	8.597		

CALIBRATION OF COMPONENT NO2

Method: AnionsIC2-120921.mtw
 Equation: $Q = 0.0463697 \cdot A + 4.1508$
 RSD: 4.769 %
 Correlation coefficient: 0.998759

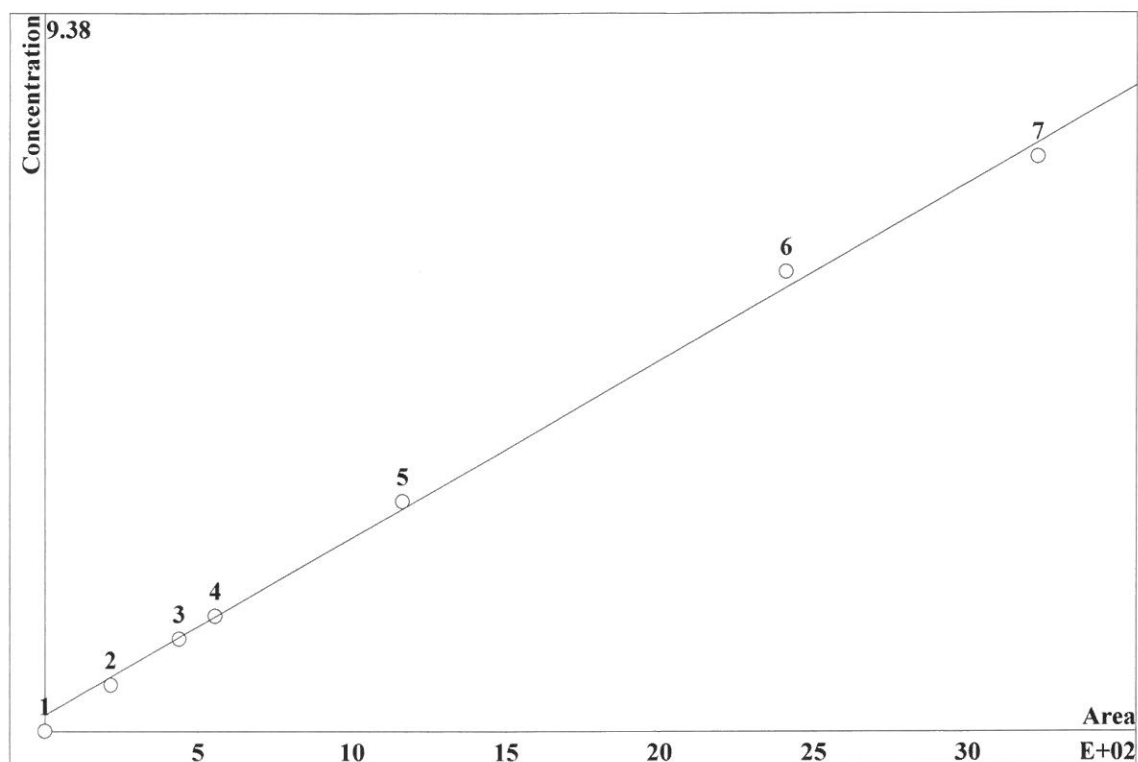

K3 = 0 K2 = 0 K1 = 0.0463697 K0 = 4.1508

Base: Area

Ref.channel: chl

ISTD:


Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used File
1	0	0	0	0	0	0
2	13.47	215.8	0.6	20	10.39	
3	27.11	439.2	1.2	20	10.39	
4	34.69	553.8	1.5	20	10.39	
5	72	1162	3	20	10.39	
6	144.2	2408	6	20	10.39	
7	194.5	3224	7.5	20	10.39	

CALIBRATION OF COMPONENT BR-

Method: AnionsIC2-120921.mtw
 Equation: $Q = 0.237959 \cdot A + 15.2141$
 RSD: 5.097 %
 Correlation coefficient: 0.998583

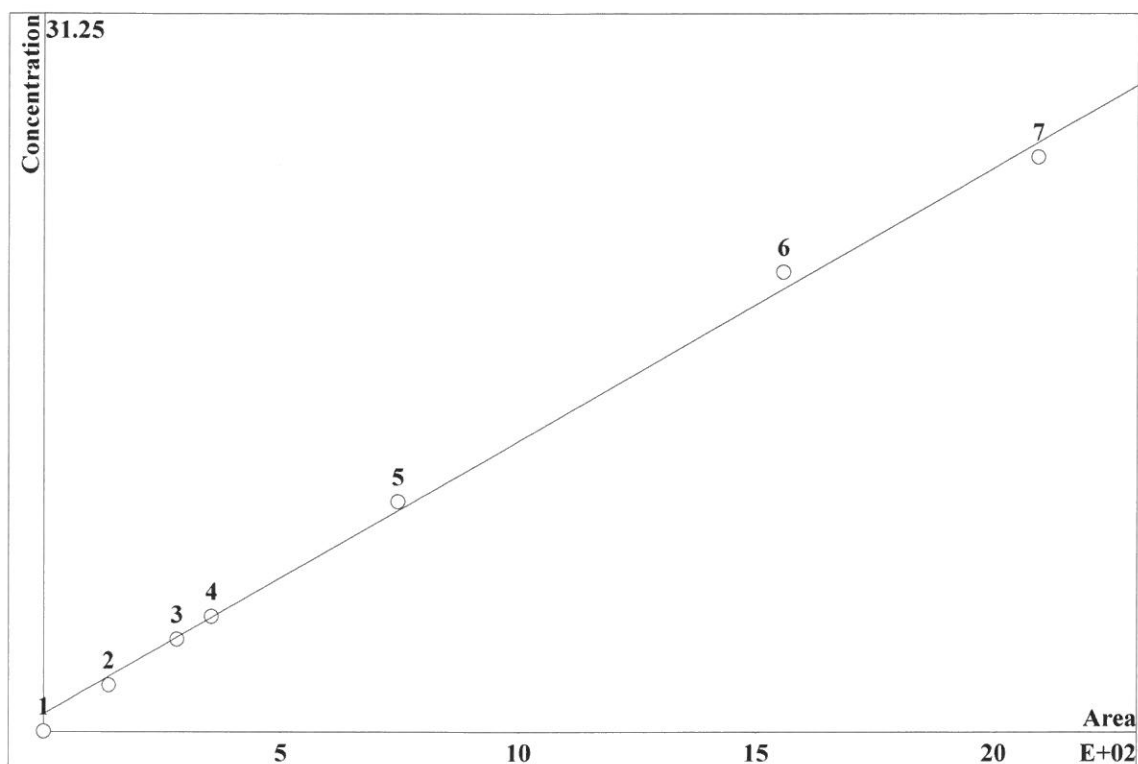

K3 = 0 K2 = 0 K1 = 0.237959 K0 = 15.2141

Base: Area

Ref.channel: chl

ISTD:


Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	7.293	137.2	2	20	14.07		
3	14.99	281.3	4	20	14.07		
4	18.97	353.5	5	20	14.07		
5	39.95	744.5	10	20	14.07		
6	82.63	1556	20	20	14.07		
7	109.5	2091	25	20	14.07		

CALIBRATION OF COMPONENT NO3

Method: AnionsIC2-120921.mtw
 Equation: $Q = 0.0408801 \cdot A + 3.90365$
 RSD: 5.579 %
 Correlation coefficient: 0.998302

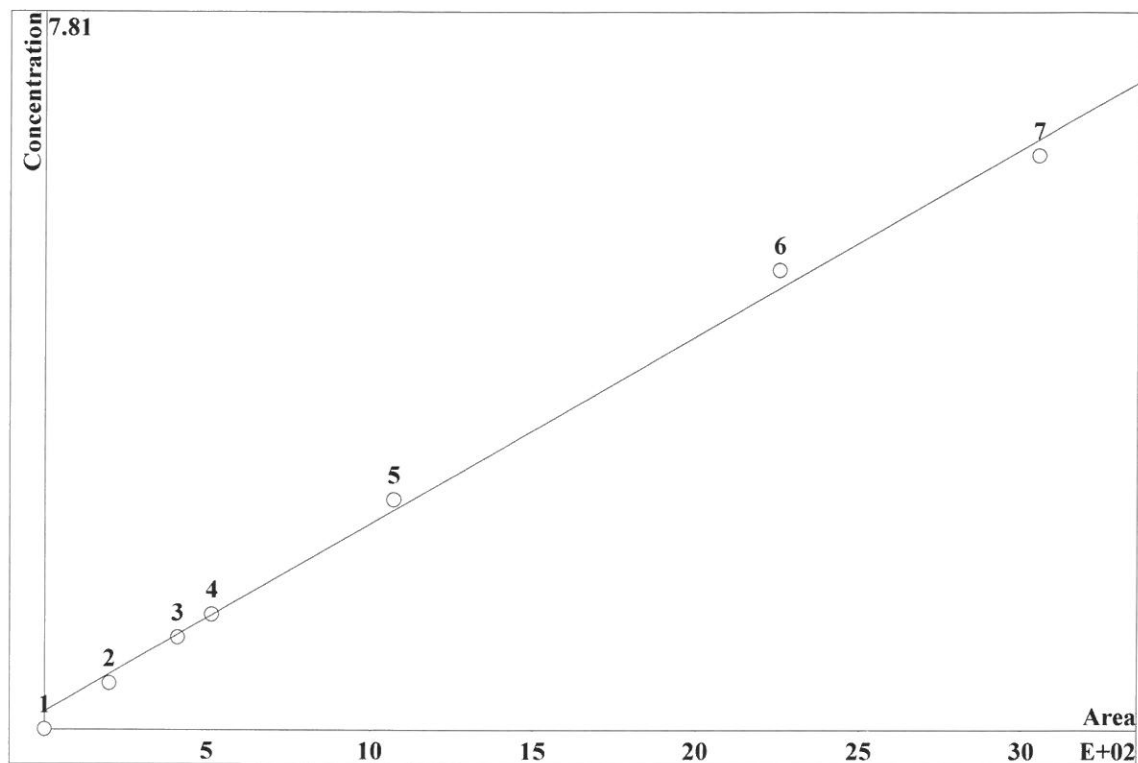

K3 = 0 K2 = 0 K1 = 0.0408801 K0 = 3.90365

Base: Area

Ref.channel: ch1

ISTD:

Formula: Linear


Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used File
1	0	0	0	0	0	0
2	9.019	200.2	0.5	20	14.73	
3	18.5	410.7	1	20	14.73	
4	23.37	514.5	1.25	20	14.73	
5	49.41	1072	2.5	20	14.73	
6	105.7	2255	5	20	14.73	
7	144.5	3048	6.25	20	14.73	

Ç

CALIBRATION OF COMPONENT HPO4

Method: AnionsIC2-120921.mtw
 Equation: $Q = 0.0701699 \cdot A - 10.6431$
 RSD: 3.686 %
 Correlation coefficient: 0.999259

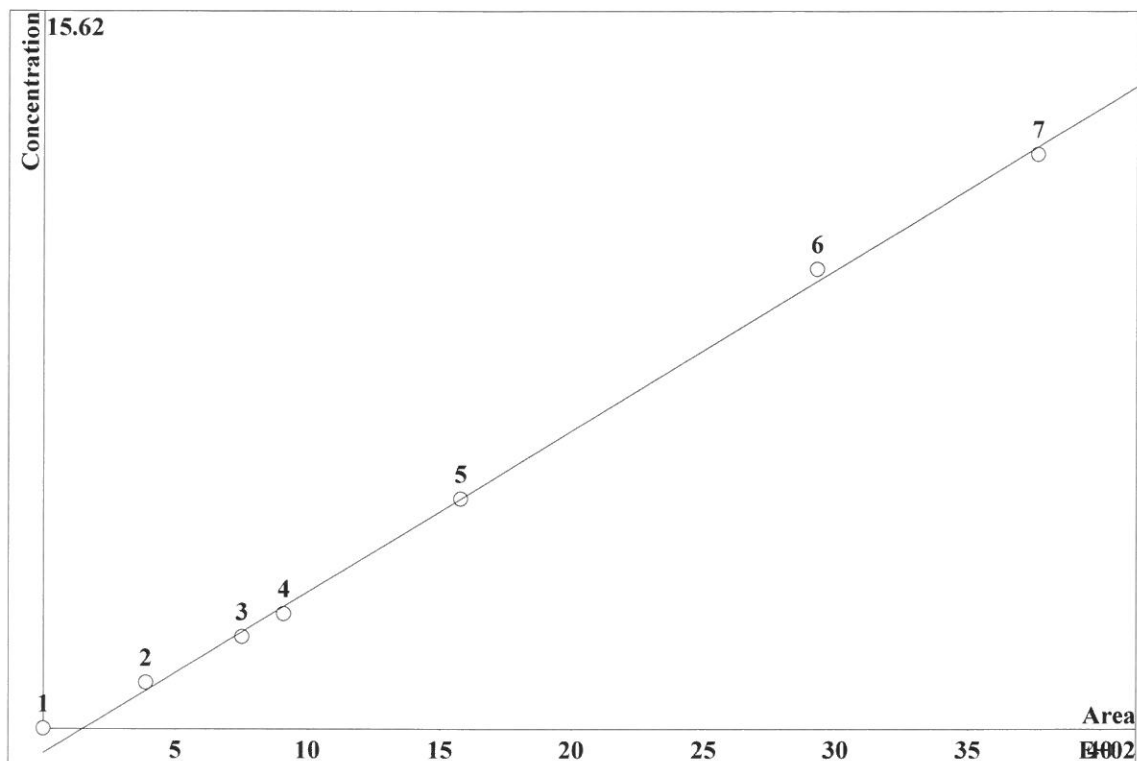

K3 = 0 K2 = 0 K1 = 0.0701699 K0 = -10.6431

Base: Area

Ref.channel: chl

ISTD:


Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used File
1	0	0	0	0	0	0
2	10.05	388.5	1	20	20.23	
3	20.81	753.1	2	20	20.23	
4	25.7	910.8	2.5	20	20.23	
5	46.35	1576	5	20	20.23	
6	92.48	2926	10	20	20.23	
7	121.9	3761	12.5	20	20.23	

CALIBRATION OF COMPONENT SO4

Method: AnionsIC2-120921.mtw
 Equation: $Q = 0.133229 \cdot A + 26.5837$
 RSD: 6.118 %
 Correlation coefficient: 0.997958

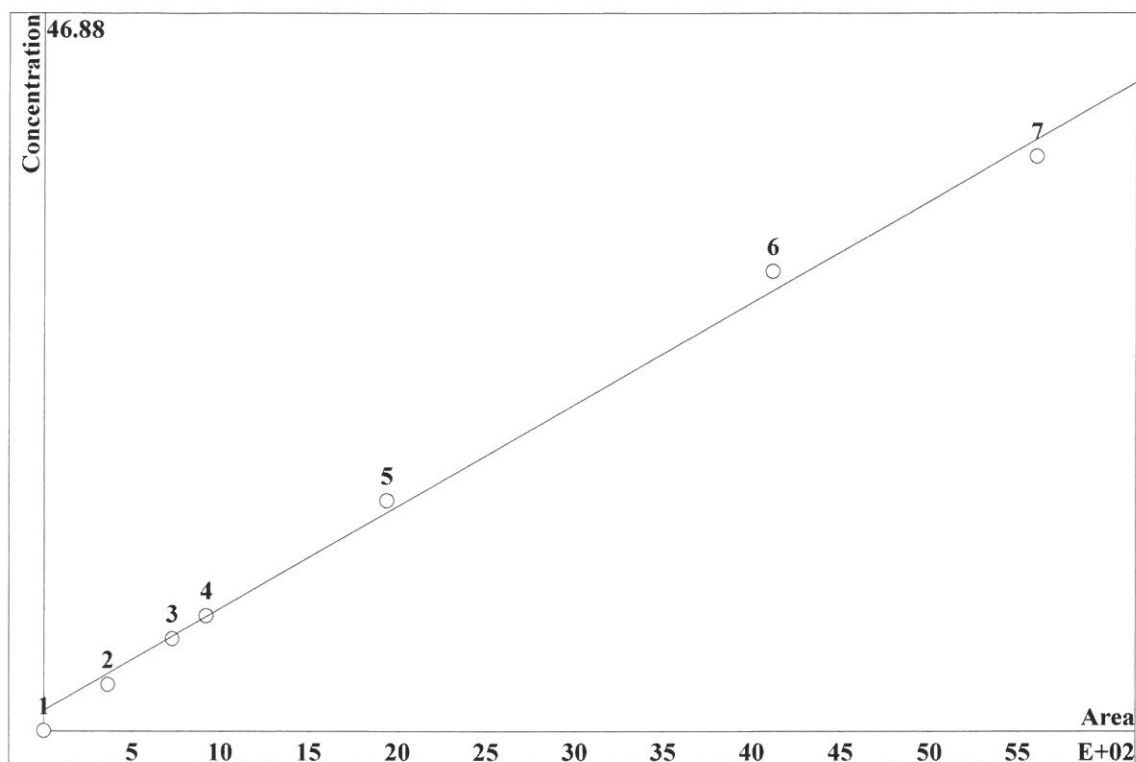

K3 = 0 K2 = 0 K1 = 0.133229 K0 = 26.5837

Base: Area

Ref.channel: chl

ISTD:

Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1		0	0	0	0		0
2	13.09	362.9	3	20	22.81		
3	26.62	730.4	6	20	22.81		
4	33.78	921	7.5	20	22.81		
5	72.28	1937	15	20	22.81		
6	156.3	4113	30	20	22.81		
7	213.9	5600	37.5	20	22.81		

Report date: 12/9/2021 3:52:10 PM
Printed by: wet


Ident: STD1
Analysis from: 12/9/2021 10:57:18 AM
File: _2021-12-09_

Last save: 12/9/2021 2:24:50 PM

Method: AnionsIC2-120921.mtw
Run operator: wet
Analysis number: 29300

Last save: 12/9/2021 1:46:

SAMPLE:
: IZ/AP
Vial number: 2
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

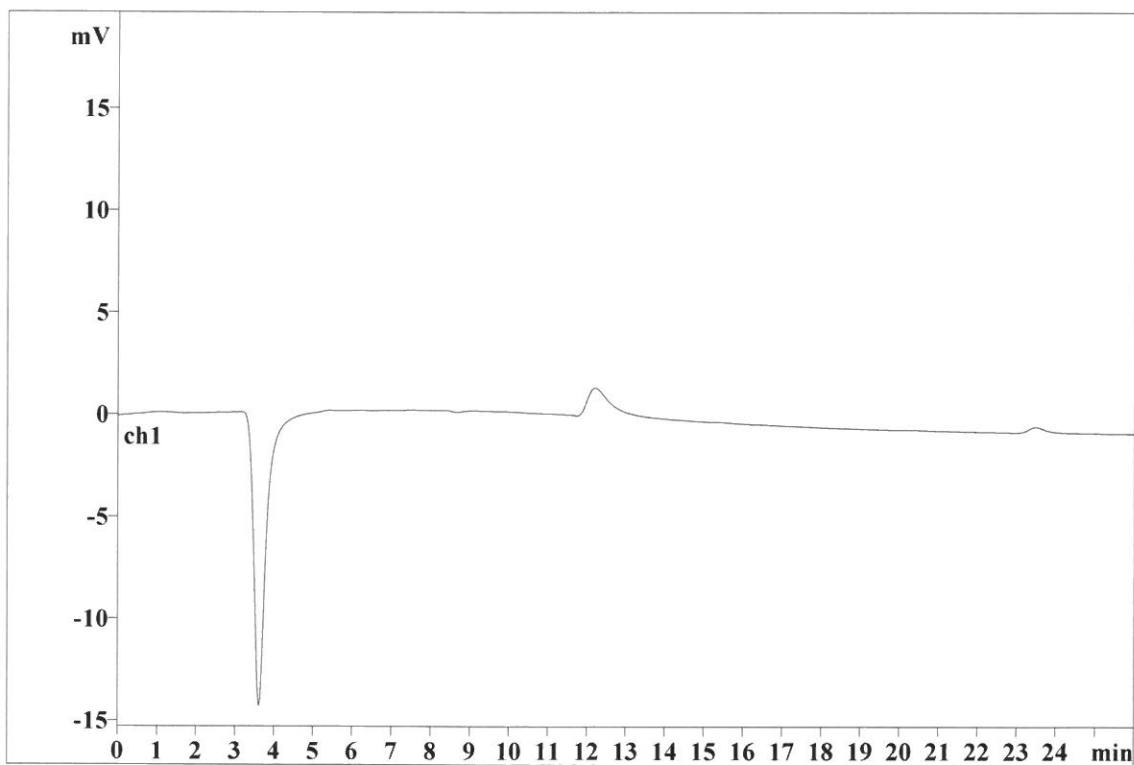

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 12/9/2021 3:52:28 PM
Printed by: wet


Ident: STD2
Analysis from: 12/9/2021 11:25:57 AM
File: _2021-12-09_

Last save: 12/9/2021 2:24:50 PM

Method: AnionsIC2-120921.mtw
Run operator: wet
Analysis number: 29301

Last save: 12/9/2021 1:46:

SAMPLE:
: IZ/AP
Vial number: 3
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

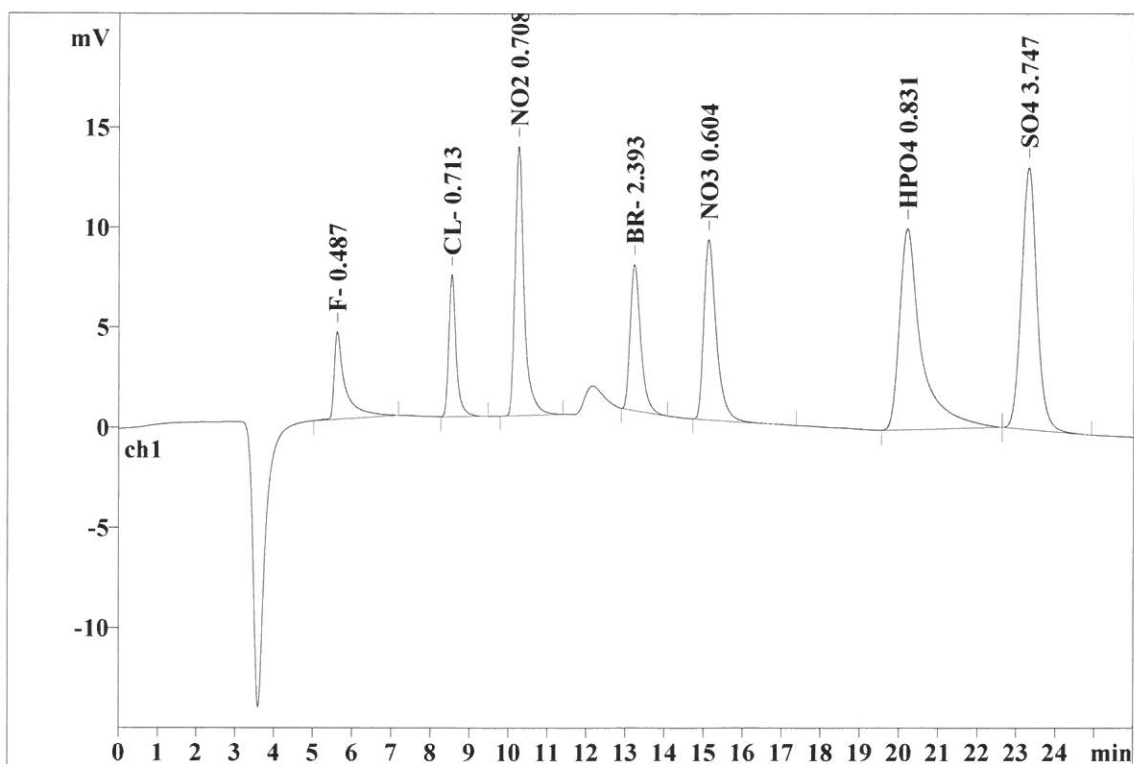

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.62	0.223	4.36	6.78	85.317	5.74
2	8.52	0.191	7.09	11.02	95.251	6.41
3	10.24	0.224	13.46	20.91	215.827	14.53
4	13.21	0.280	7.29	11.33	137.190	9.24
5	15.11	0.325	9.02	14.01	200.206	13.48
6	20.18	0.488	10.05	15.61	388.518	26.16
7	23.29	0.418	13.09	20.33	362.918	24.44
7	26.00	0.307	64.36	99.98	1485.227	100.00

This report has been created by IC Net
METROHM LTD

Report date: 12/9/2021 3:52:38 PM
Printed by: wet


Ident: STD3
Analysis from: 12/9/2021 11:54:35 AM
File: _2021-12-09_

Last save: 12/9/2021 2:24:50 PM

Method: AnionsIC2-120921.mtw
Run operator: wet
Analysis number: 29302

Last save: 12/9/2021 1:46:

SAMPLE:
: IZ/AP
Vial number: 4
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

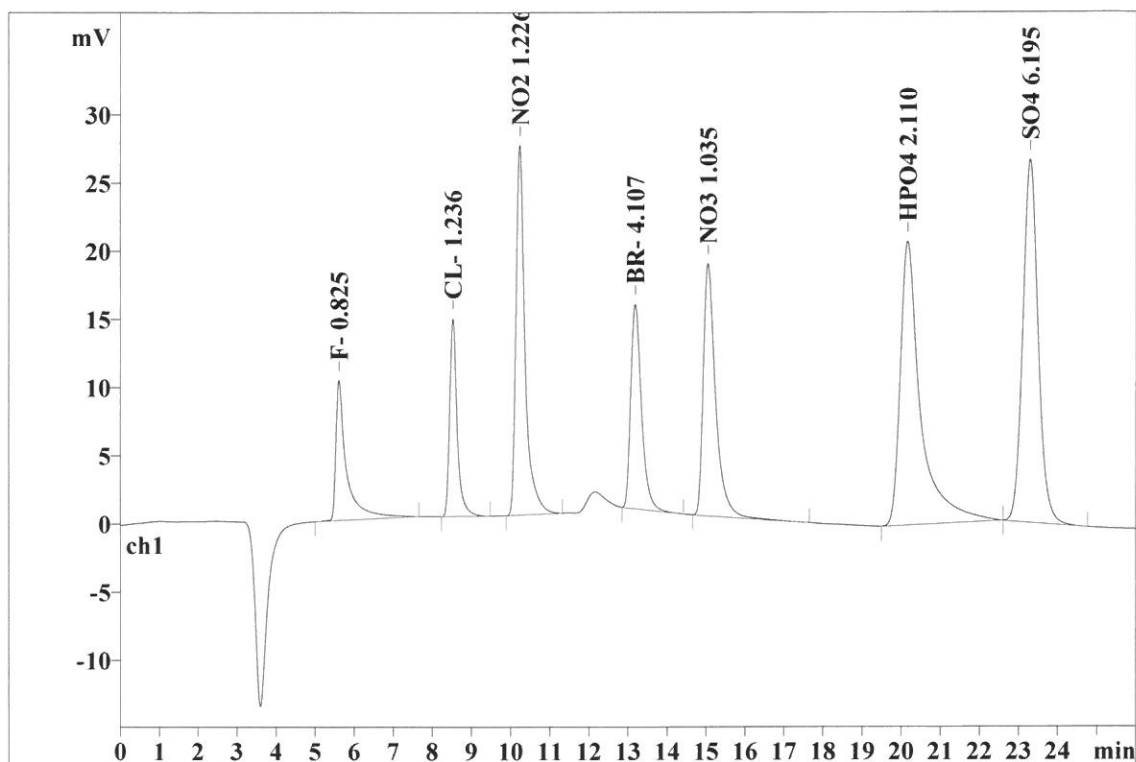

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.61	0.214	10.27	7.74	195.856	6.52
2	8.51	0.190	14.50	10.92	194.161	6.46
3	10.22	0.226	27.10	20.41	439.163	14.62
4	13.17	0.278	14.99	11.29	281.277	9.36
5	15.04	0.321	18.50	13.93	410.745	13.67
6	20.15	0.462	20.81	15.67	753.136	25.06
7	23.28	0.414	26.62	20.04	730.404	24.31
7	26.00	0.300	132.78	100.00	3004.742	100.00

This report has been created by IC Net
METROHM LTD

Report date: 12/9/2021 3:52:47 PM
Printed by: wet


Ident: STD4
Analysis from: 12/9/2021 12:23:13 PM
File: _2021-12-09_

Last save: 12/9/2021 2:24:50 PM

Method: AnionsIC2-120921.mtw
Run operator: wet
Analysis number: 29303

Last save: 12/9/2021 1:46:

SAMPLE:
: IZ/AP
Vial number: 5
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

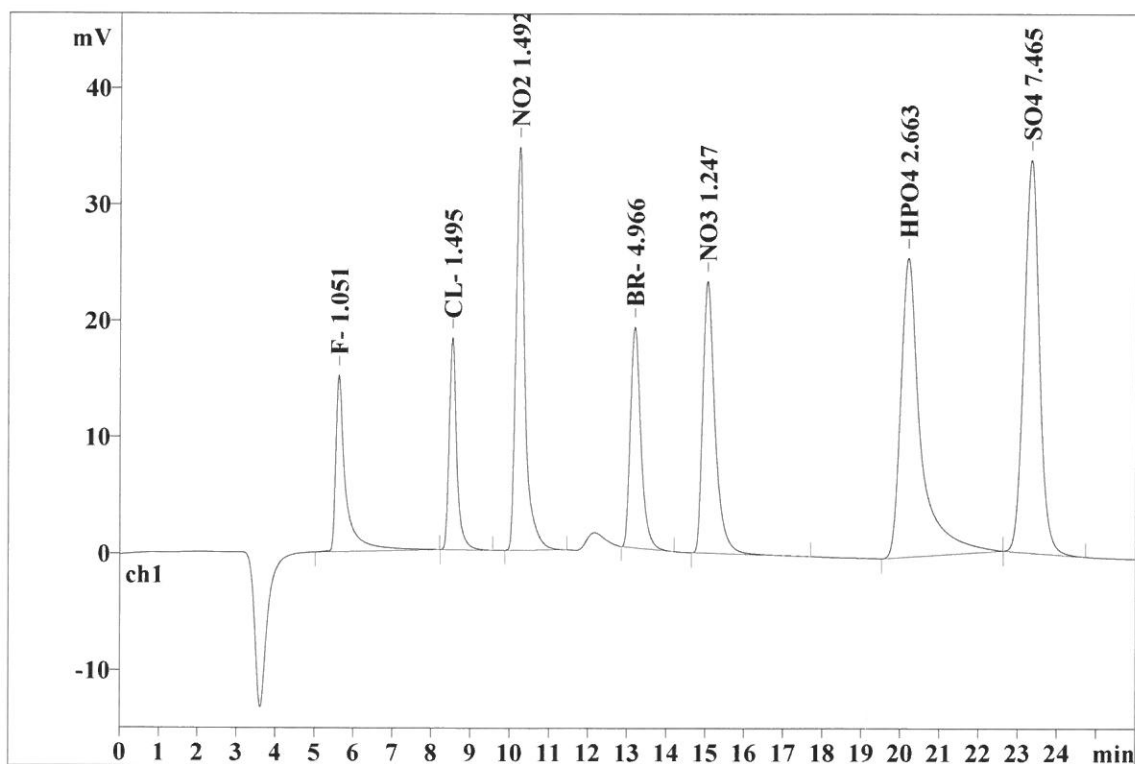

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.61	0.205	15.18	8.93	269.876	7.16
2	8.52	0.190	18.21	10.72	243.290	6.46
3	10.22	0.223	34.69	20.42	553.825	14.70
4	13.17	0.277	18.97	11.16	353.482	9.38
5	15.03	0.320	23.37	13.76	514.474	13.66
6	20.17	0.454	25.70	15.13	910.760	24.18
7	23.31	0.411	33.78	19.88	921.024	24.45
7	26.00	0.297	169.90	100.00	3766.731	100.00

This report has been created by IC Net
METROHM LTD

Report date: 12/9/2021 3:53:12 PM
Printed by: wet


Ident: STD5
Analysis from: 12/9/2021 12:51:52 PM
File: _2021-12-09_

Last save: 12/9/2021 2:24:50 PM

Method: AnionsIC2-120921.mtw
Run operator: wet
Analysis number: 29304

Last save: 12/9/2021 1:46:

SAMPLE:
: IZ/AP
Vial number: 6
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

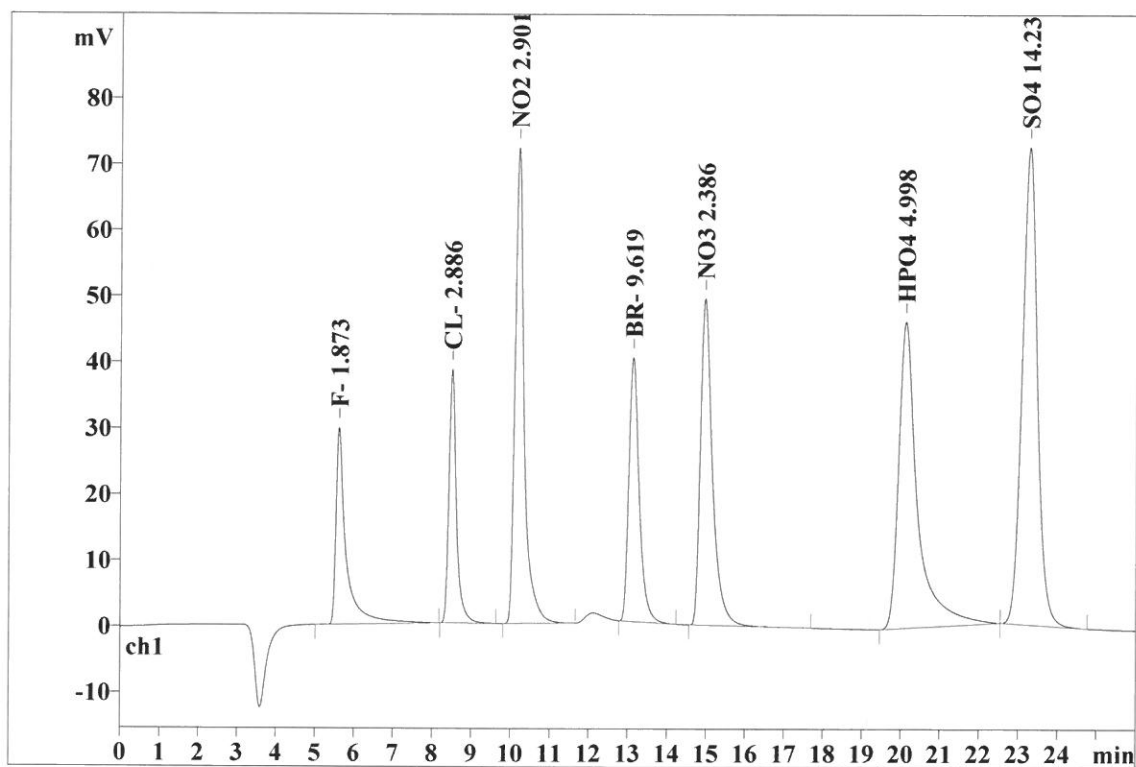

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.61	0.207	29.78	8.55	538.229	7.14
2	8.49	0.186	38.42	11.03	506.890	6.73
3	10.18	0.224	72.00	20.68	1161.914	15.42
4	13.12	0.276	39.95	11.47	744.503	9.88
5	14.95	0.314	49.41	14.19	1071.927	14.22
6	20.10	0.438	46.35	13.31	1576.092	20.91
7	23.24	0.403	72.28	20.76	1937.297	25.70
7	26.00	0.293	348.18	100.00	7536.852	100.00

This report has been created by IC Net
METROHM LTD

Report date: 12/9/2021 3:53:19 PM
Printed by: wet


Ident: STD6
Analysis from: 12/9/2021 1:20:30 PM
File: _2021-12-09_

Last save: 12/9/2021 2:24:50 PM

Method: AnionsIC2-120921.mtw
Run operator: wet
Analysis number: 29305

Last save: 12/9/2021 1:46:

SAMPLE:
: IZ/AP
Vial number: 7
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

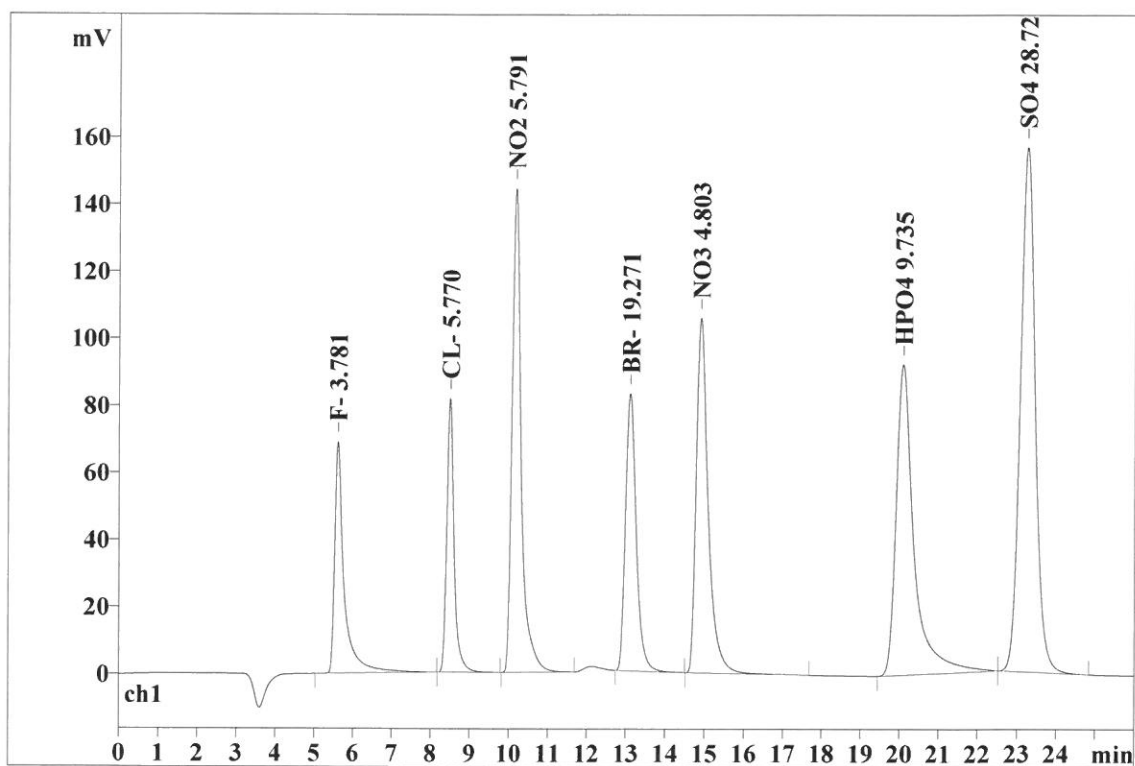

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.61	0.201	69.12	9.44	1161.907	7.51
2	8.48	0.183	81.58	11.14	1053.305	6.81
3	10.16	0.235	144.18	19.70	2408.204	15.56
4	13.10	0.281	82.62	11.29	1555.770	10.05
5	14.89	0.308	105.74	14.44	2254.516	14.57
6	20.07	0.416	92.48	12.63	2926.310	18.91
7	23.23	0.396	156.29	21.35	4113.171	26.58
7	26.00	0.288	732.02	100.00	15473.184	100.00

This report has been created by IC Net
METROHM LTD

Report date: 12/9/2021 3:53:27 PM
Printed by: wet


Ident: STD7
Analysis from: 12/9/2021 1:49:09 PM
File: _2021-12-09_

Last save: 12/9/2021 2:24:50 PM

Method: AnionsIC2-120921.mtw
Run operator: wet
Analysis number: 29306

Last save: 12/9/2021 1:46:

SAMPLE:
: IZ/AP
Vial number: 8
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

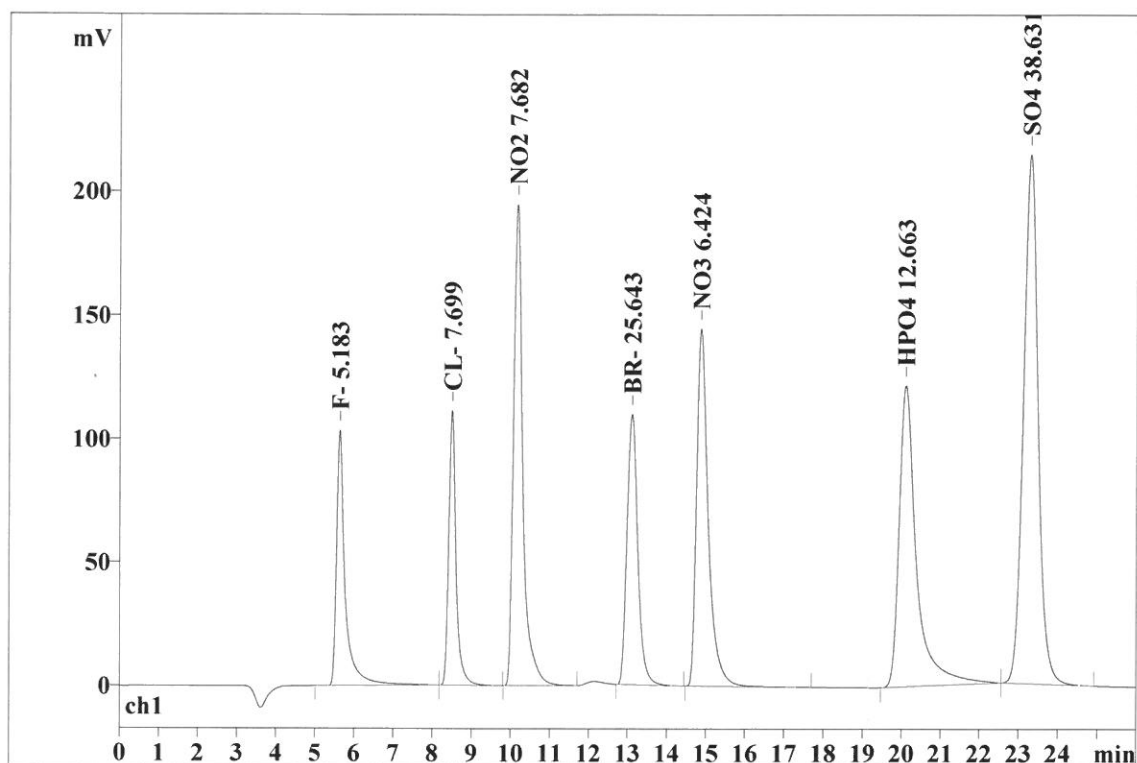

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.62	0.196	103.37	10.35	1620.374	7.80
2	8.49	0.181	111.11	11.13	1418.772	6.83
3	10.15	0.233	194.51	19.48	3224.034	15.53
4	13.10	0.287	109.49	10.96	2091.344	10.07
5	14.86	0.305	144.50	14.47	3047.582	14.68
6	20.09	0.408	121.88	12.20	3760.981	18.11
7	23.27	0.394	213.86	21.41	5599.567	26.97
7	26.00	0.286	998.71	100.00	20762.654	100.00

This report has been created by IC Net
METROHM LTD

Report date: 12/9/2021 3:53:42 PM
Printed by: wet


Ident: ICV
Analysis from: 12/9/2021 2:25:36 PM
File: _2021-12-09_

Last save: 12/9/2021 2:51:37 PM

Method: AnionsIC2-120921.mtw
Run operator: wet
Analysis number: 29307

Last save: 12/9/2021 2:15:

SAMPLE:
: IZ/AP
Vial number: 9
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

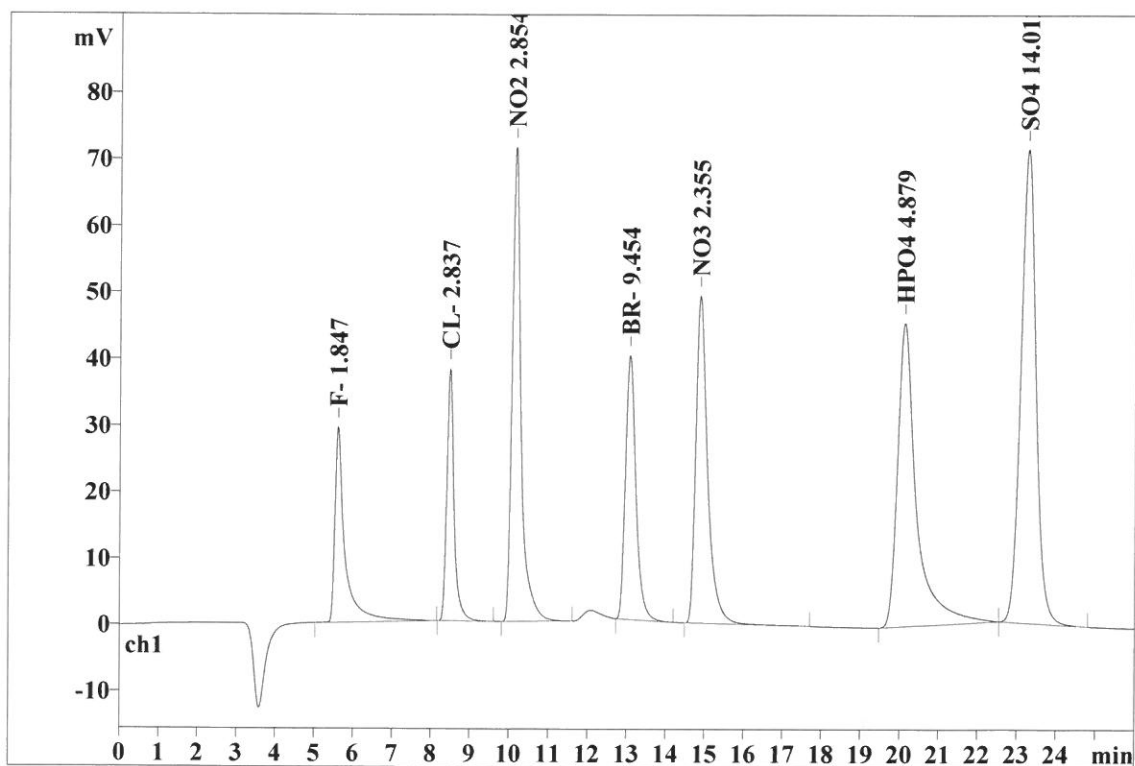

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.60	0.206	29.42	8.54	530.019	7.16
2	8.47	0.185	37.96	11.02	497.623	6.72
3	10.14	0.223	71.31	20.70	1141.595	15.42
4	13.06	0.273	39.70	11.52	730.638	9.87
5	14.86	0.311	49.22	14.29	1056.637	14.27
6	20.10	0.436	45.63	13.25	1542.317	20.83
7	23.24	0.402	71.22	20.67	1903.967	25.72
7	26.00	0.291	344.46	100.00	7402.796	100.00

This report has been created by IC Net
METROHM LTD

Report date: 12/9/2021 3:53:49 PM
Printed by: wet


Ident: ICB
Analysis from: 12/9/2021 2:55:34 PM
File: _2021-12-09_

Last save: 12/9/2021 3:21:34 PM

Method: AnionsIC2-120921.mtw
Run operator: wet
Analysis number: 29308

Last save: 12/9/2021 2:15:

SAMPLE:
: IZ/AP
Vial number: 10
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

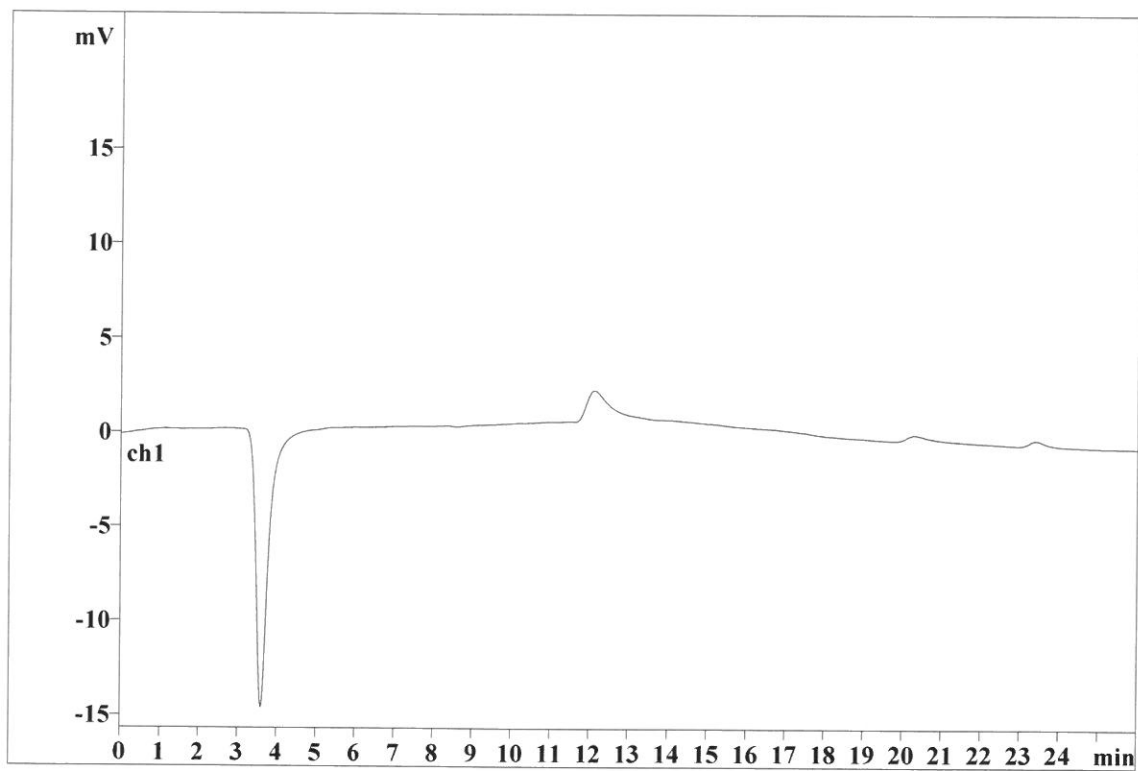

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 12/23/2021 1:57:42 PM
Printed by: wet


Ident: CCV
Analysis from: 12/23/2021 8:54:47 AM
File: _2021-12-23_

Last save: 12/23/2021 9:32:15 AM

Method: AnionsIC2-120921.mtw
Run operator: wet
Analysis number: 29524

Last save: 12/21/2021 10:1

SAMPLE:
: IZ/AP
Vial number: 11
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

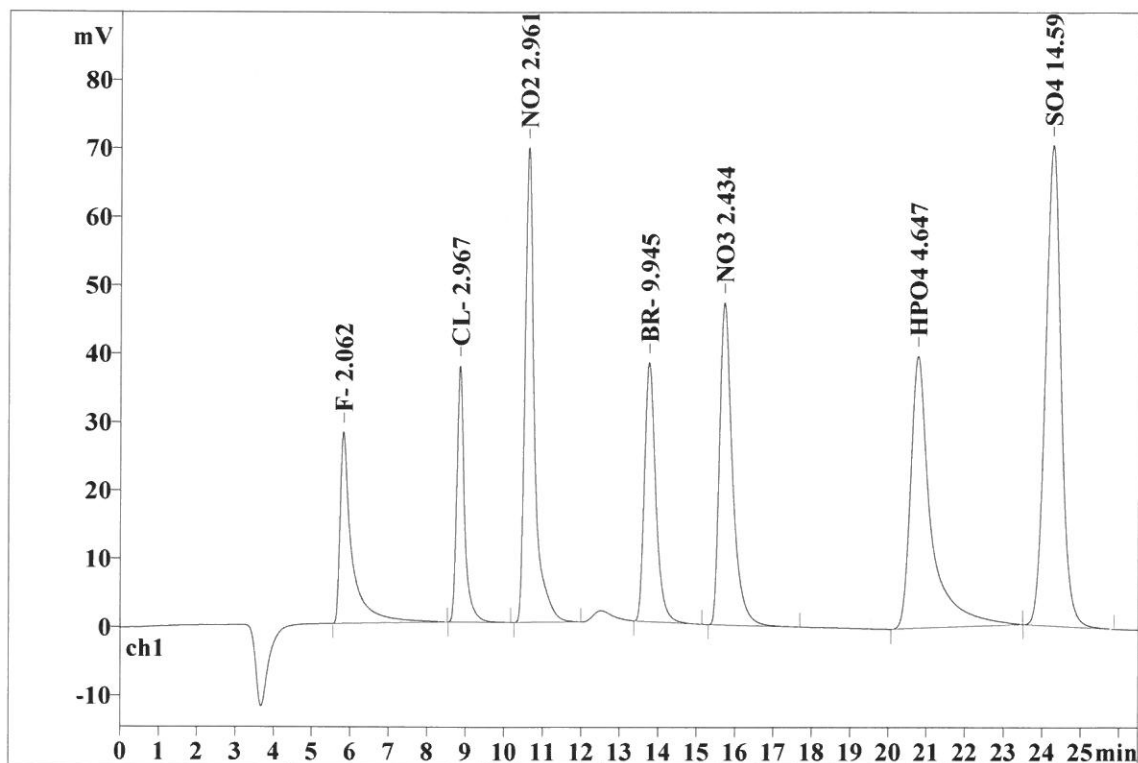

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.81	0.245	28.01	8.49	600.174	7.85
2	8.84	0.194	37.51	11.37	522.163	6.83
3	10.61	0.234	69.41	21.03	1187.600	15.53
4	13.75	0.302	37.90	11.48	771.891	10.10
5	15.70	0.338	47.13	14.28	1095.297	14.33
6	20.76	0.469	39.79	12.06	1476.196	19.31
7	24.24	0.427	70.25	21.29	1991.727	26.05
7	26.50	0.316	330.00	100.00	7645.048	100.00

This report has been created by IC Net
METROHM LTD

Report date: 12/23/2021 1:57:52 PM
Printed by: wet


Ident: CCB
Analysis from: 12/23/2021 9:23:55 AM
File: _2021-12-23_

Last save: 12/23/2021 9:50:25 AM

Method: AnionsIC2-120921.mtw
Run operator: wet
Analysis number: 29525

Last save: 12/21/2021 10:1

SAMPLE:
: IZ/AP
Vial number: 12
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

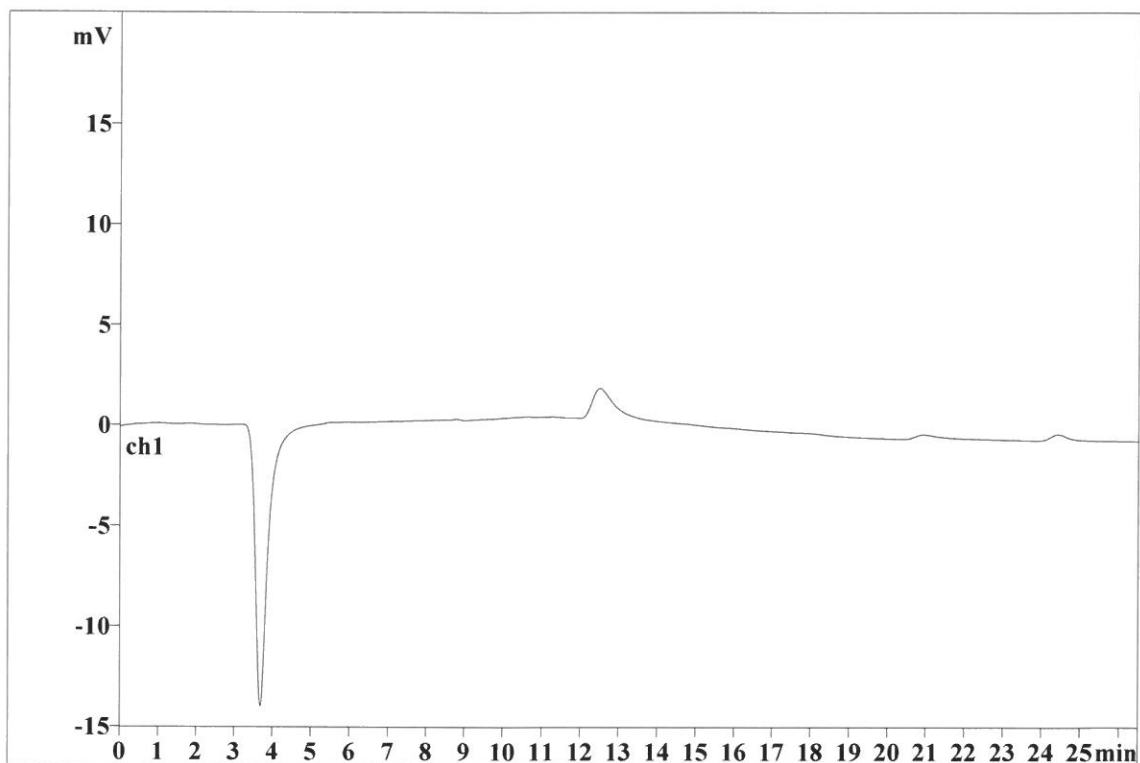

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 12/23/2021 1:58:02 PM
Printed by: wet


Ident: LB117940BLW
Analysis from: 12/23/2021 9:53:04 AM
File: _2021-12-23_

Last save: 12/23/2021 11:01:33 AM

Method: AnionsIC2-120921.mtw
Run operator: wet
Analysis number: 29526

Last save: 12/21/2021 10:1

SAMPLE:
: IZ/AP
Vial number: 13
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

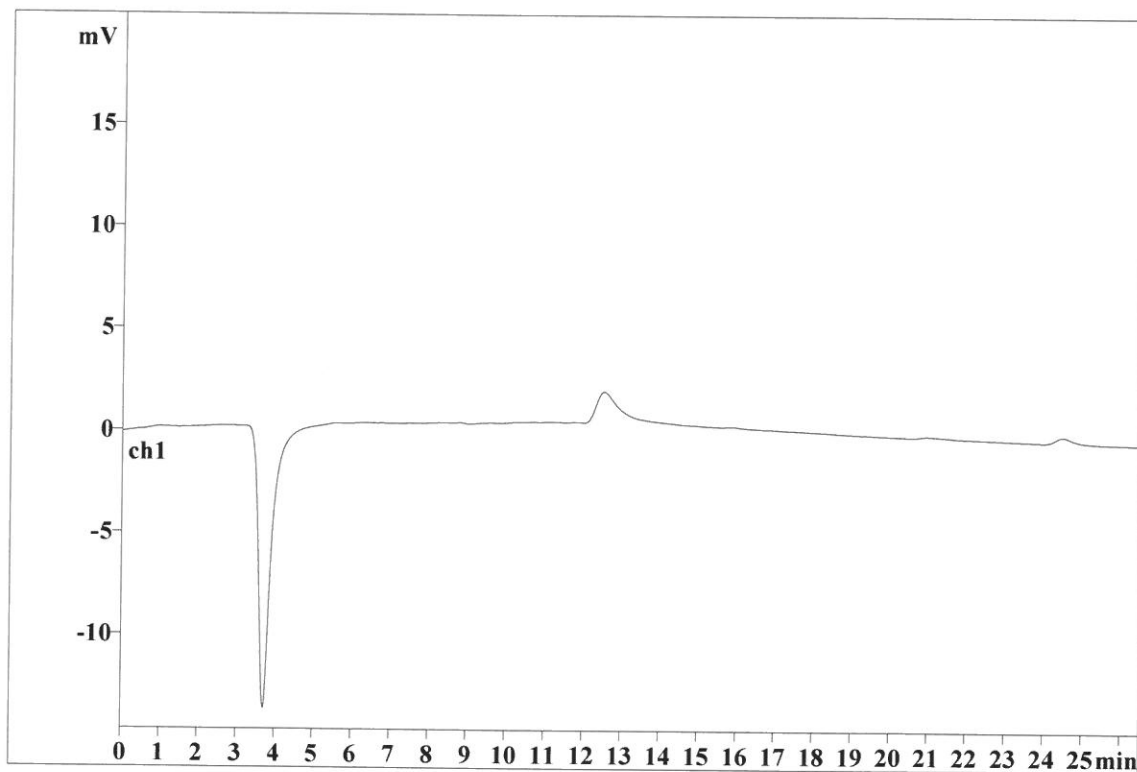

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 12/23/2021 1:58:11 PM
Printed by: wet


Ident: LB117940BSW
Analysis from: 12/23/2021 10:22:13 AM
File: _2021-12-23_

Last save: 12/23/2021 11:01:33 AM

Method: AnionsIC2-120921.mtw
Run operator: wet
Analysis number: 29527

Last save: 12/21/2021 10:1

SAMPLE:
: IZ/AP
Vial number: 14
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

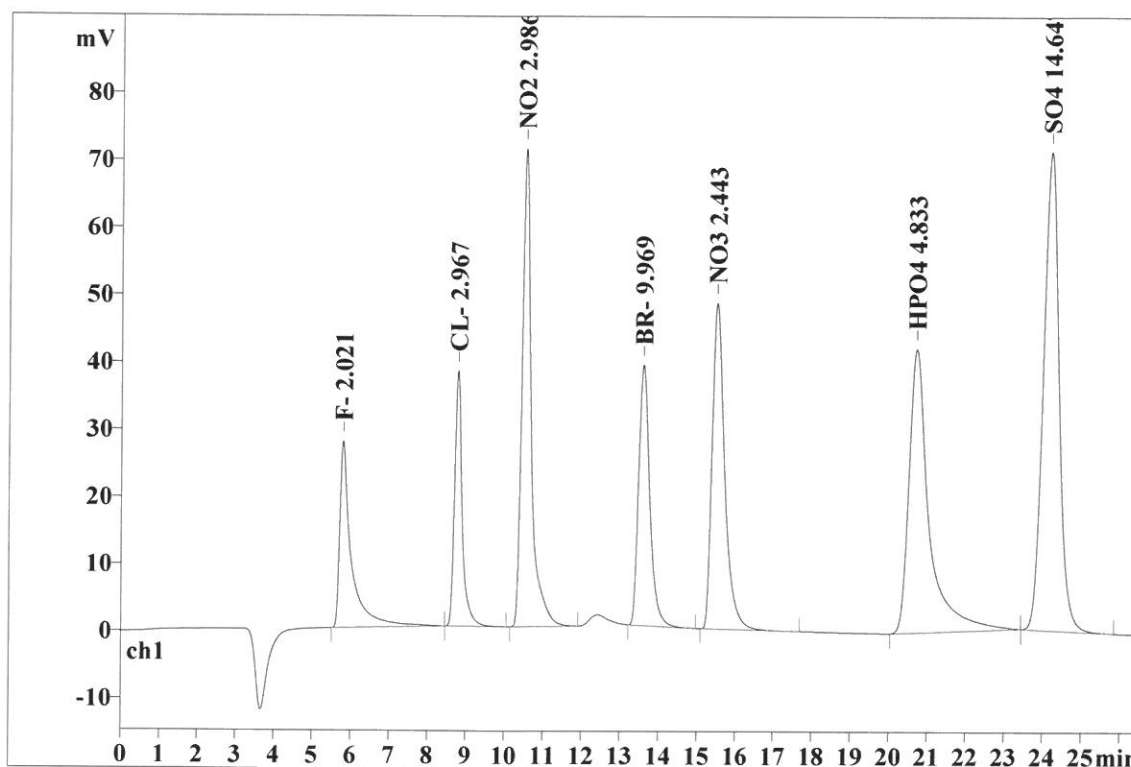

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.79	0.241	27.72	8.22	586.830	7.61
2	8.77	0.192	37.99	11.27	522.277	6.77
3	10.51	0.231	71.03	21.06	1198.308	15.54
4	13.58	0.297	38.77	11.50	773.902	10.04
5	15.49	0.330	48.45	14.37	1099.622	14.26
6	20.69	0.463	42.16	12.50	1529.138	19.83
7	24.16	0.424	71.07	21.08	1999.241	25.93
7	26.50	0.311	337.19	100.00	7709.318	100.00

This report has been created by IC Net
METROHM LTD

Report date: 12/23/2021 1:58:23 PM
Printed by: wet


Ident: M5205-01X100
Analysis from: 12/23/2021 10:53:24 AM
File: _2021-12-23_

Last save: 12/23/2021 11:23:37 AM

Method: AnionsIC2-120921.mtw
Run operator: wet
Analysis number: 29528

Last save: 12/21/2021 10:1

SAMPLE:
: IZ/AP
Vial number: 18
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

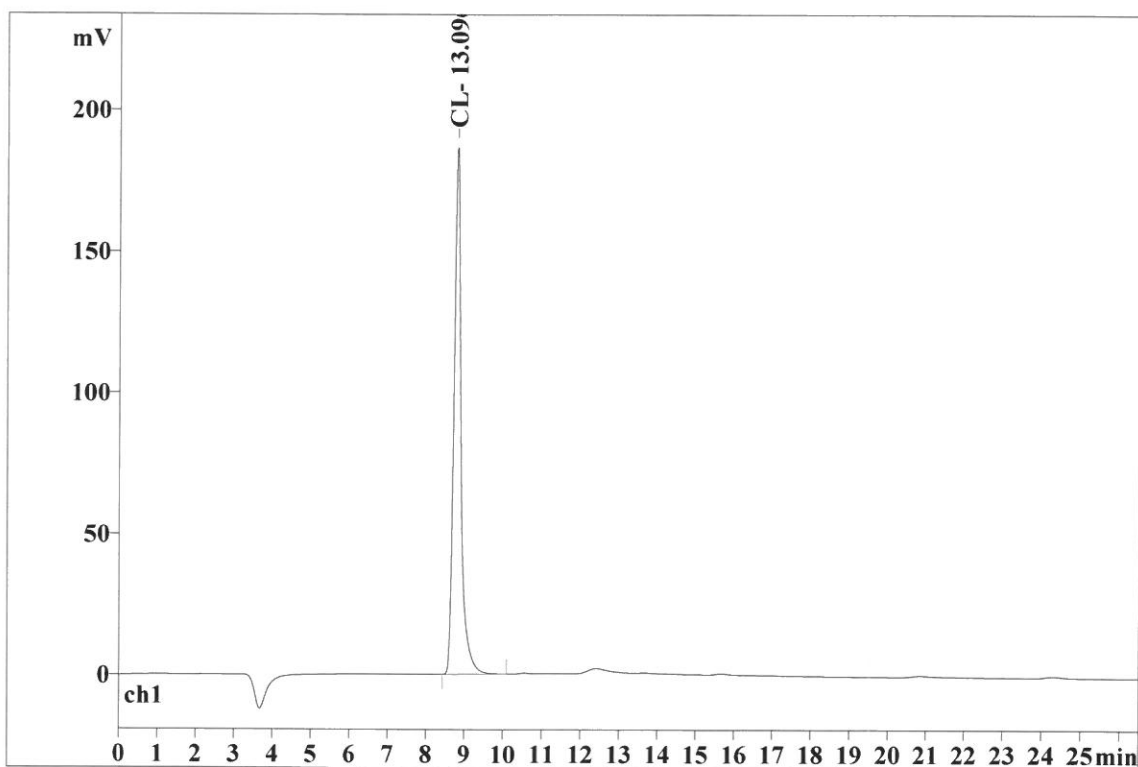

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	8.77	0.182	186.68	100.00	2441.100	100.00
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	0.00	0.000	0.00	0.00	0.000	0.00
6	0.00	0.000	0.00	0.00	0.000	0.00
7	0.00	0.000	0.00	0.00	0.000	0.00
7	26.50	0.026	186.68	100.00	2441.100	100.00

This report has been created by IC Net
METROHM LTD

Report date: 12/23/2021 1:58:34 PM
Printed by: wet


Ident: M5205-01MSX100
Analysis from: 12/23/2021 11:22:39 AM
File: _2021-12-23_

Last save: 12/23/2021 11:49:09 AM

Method: AnionsIC2-120921.mtw
Run operator: wet
Analysis number: 29529

Last save: 12/21/2021 10:1

SAMPLE:
: IZ/AP
Vial number: 19
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

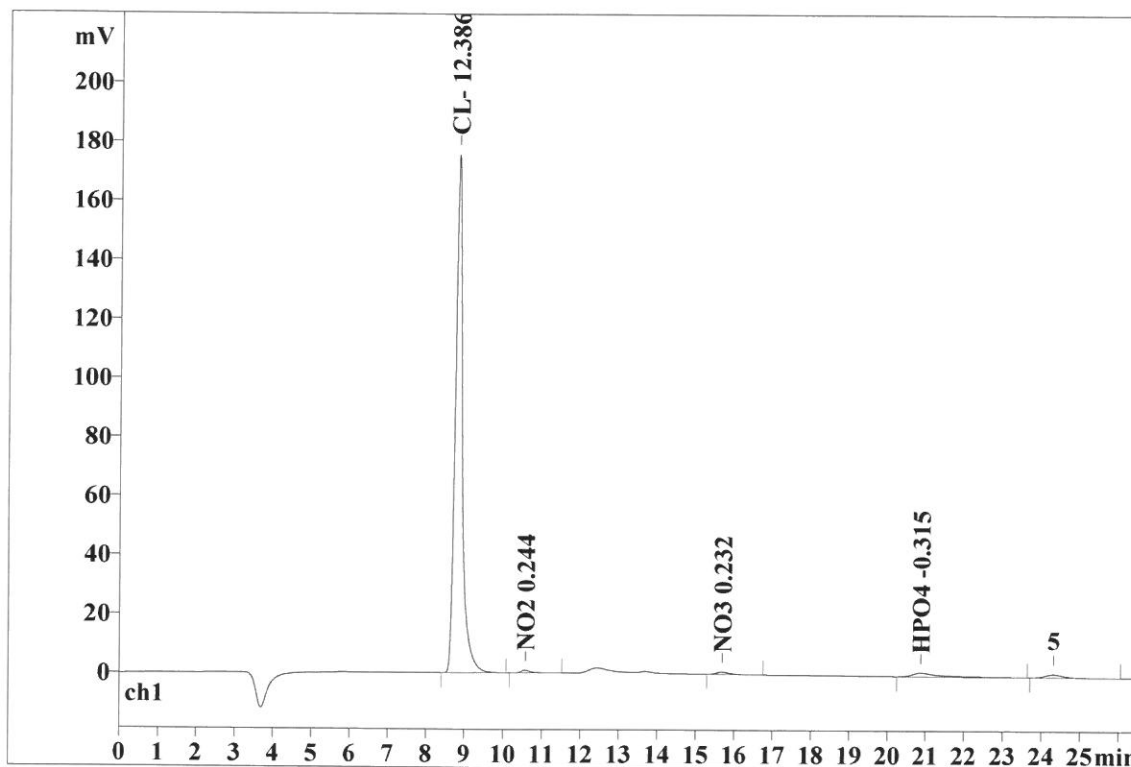

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	8.79	0.183	175.60	97.76	2306.575	94.69
3	10.57	0.231	0.90	0.50	15.600	0.64
4	0.00	0.000	0.00	0.00	0.000	0.00
5	15.69	0.351	0.76	0.42	17.780	0.73
6	20.87	0.579	1.29	0.72	61.852	2.54
7	0.00	0.000	0.00	0.00	0.000	0.00
7	26.50	0.192	178.56	99.40	2401.807	98.60

This report has been created by IC Net
METROHM LTD

Report date: 12/23/2021 1:58:46 PM
Printed by: wet


Ident: M5205-01MSDX100
Analysis from: 12/23/2021 11:51:46 AM
File: _2021-12-23_

Last save: 12/23/2021 12:18:16 PM

Method: AnionsIC2-120921.mtw
Run operator: wet
Analysis number: 29530

Last save: 12/21/2021 10:1

SAMPLE:
:
Vial number: 20
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

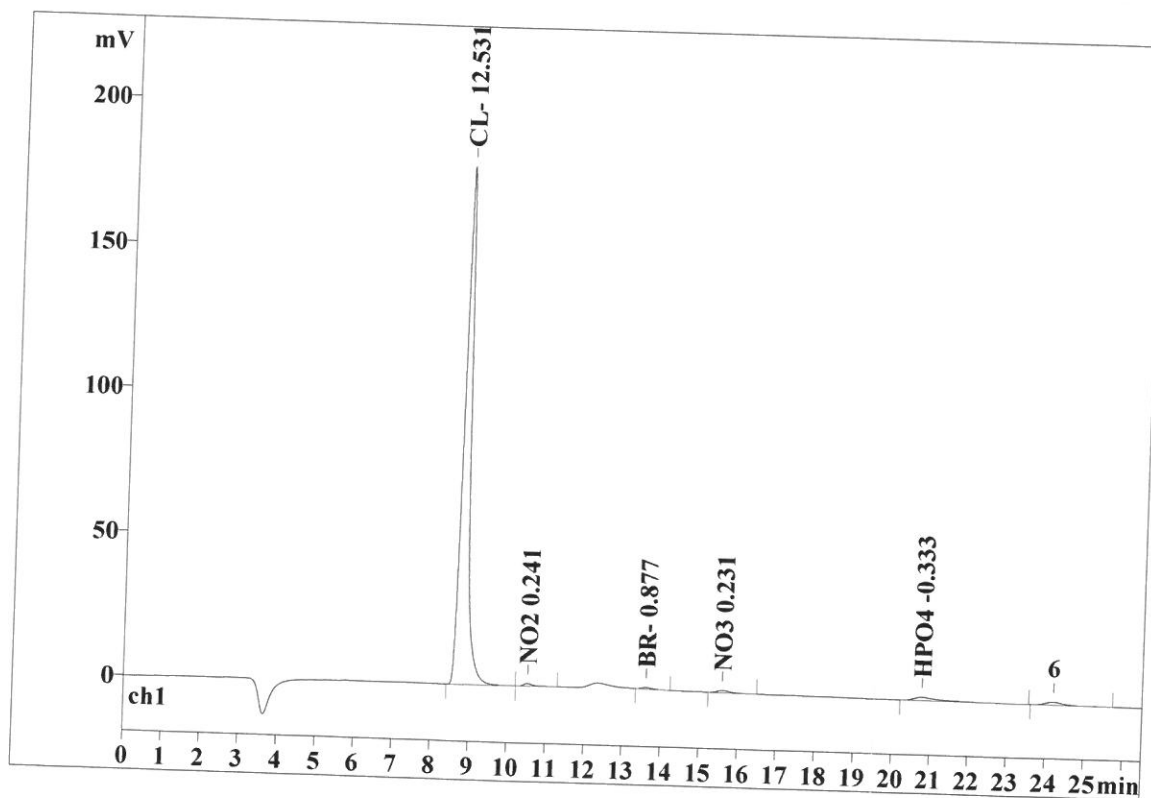

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	8.74	0.182	178.74	97.58	2334.118	94.66
3	10.52	0.229	0.90	0.49	14.618	0.59
4	13.61	0.289	0.52	0.28	9.814	0.40
5	15.59	0.344	0.77	0.42	17.482	0.71
6	20.78	0.592	1.18	0.64	56.630	2.30
7	0.00	0.000	0.00	0.00	0.000	0.00
7	26.50	0.234	182.11	99.41	2432.662	98.66

This report has been created by IC Net
METROHM LTD

Report date: 12/23/2021 1:59:05 PM
Printed by: wet


Ident: M5205-01DLX300
Analysis from: 12/23/2021 12:20:54 PM
File: _2021-12-23_

Last save: 12/23/2021 12:47:24 PM

Method: AnionsIC2-120921.mtw
Run operator: wet
Analysis number: 29531

Last save: 12/21/2021 10:1

SAMPLE:
:
Vial number: IZ/AP
Volume: 21
Dilution: 20.0 µL
Amount: 1.00
1.0000

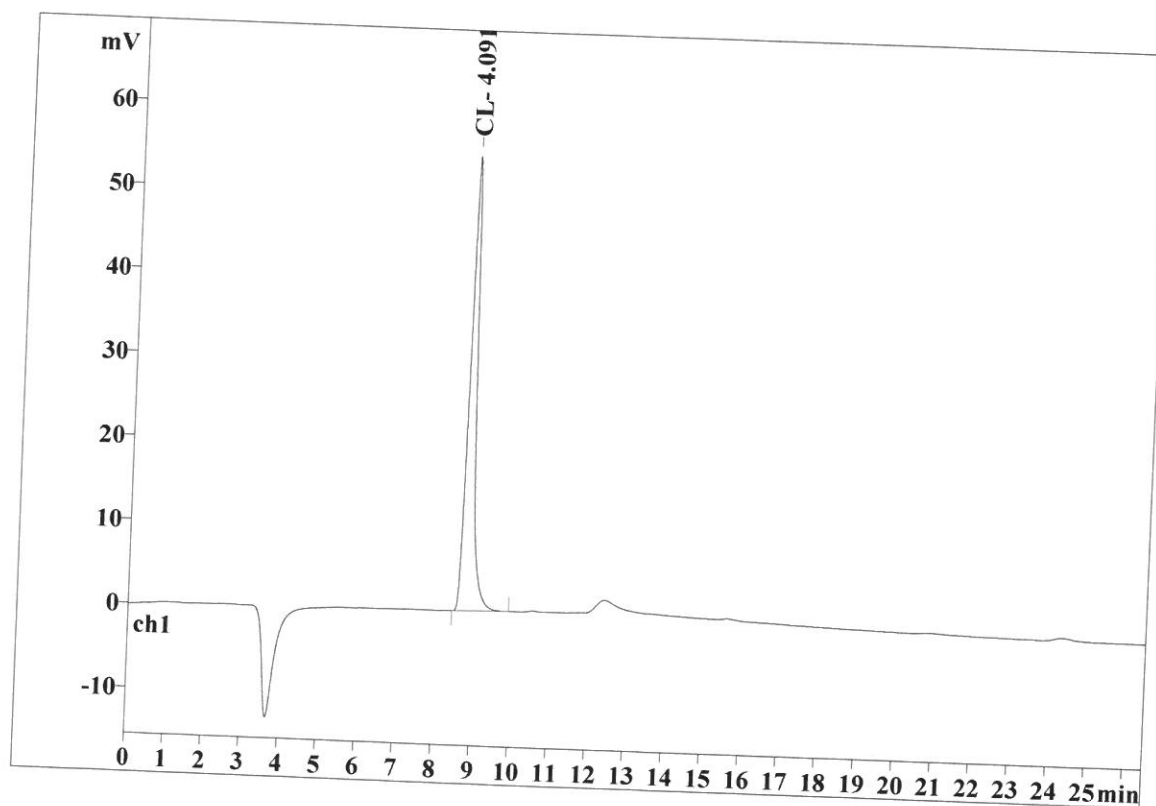

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	8.76	0.189	54.17	100.00	735.093	100.00
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	0.00	0.000	0.00	0.00	0.000	0.00
6	0.00	0.000	0.00	0.00	0.000	0.00
7	0.00	0.000	0.00	0.00	0.000	0.00
7	26.50	0.027	54.17	100.00	735.093	100.00

This report has been created by IC Net
METROHM LTD

Report date: 12/23/2021 1:59:14 PM
Printed by: wet


Ident: CCV
Analysis from: 12/23/2021 12:50:06 PM
File: _2021-12-23_

Last save: 12/23/2021 1:31:52 PM

Method: AnionsIC2-120921.mtw
Run operator: wet
Analysis number: 29532

Last save: 12/21/2021 10:1

SAMPLE:
:
Vial number: 11
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

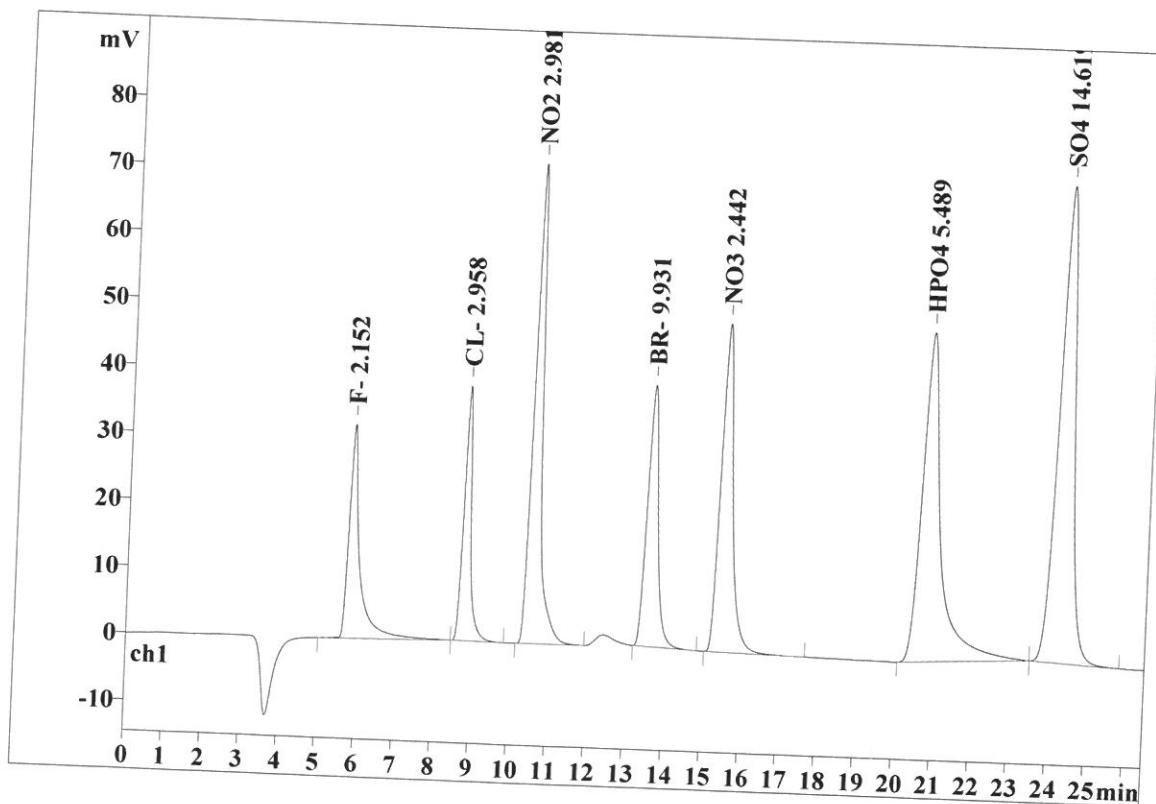

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.80	0.234	31.83	9.12	629.656	7.94
2	8.78	0.192	37.95	10.88	520.520	6.57
3	10.51	0.230	71.43	20.47	1196.103	15.09
4	13.55	0.295	38.93	11.16	770.708	9.72
5	15.45	0.328	48.87	14.00	1099.026	13.86
6	20.77	0.452	48.98	14.04	1716.195	21.65
7	24.26	0.424	70.95	20.33	1994.988	25.17
7	26.50	0.308	348.94	100.00	7927.196	100.00

This report has been created by IC Net
METROHM LTD

Report date: 12/23/2021 1:59:24 PM
Printed by: wet


Ident: CCB
Analysis from: 12/23/2021 1:19:16 PM
File: _2021-12-23_

Last save: 12/23/2021 1:45:46 PM

Method: AnionsIC2-120921.mtw
Run operator: wet
Analysis number: 29533

Last save: 12/21/2021 10:1

SAMPLE:
:
Vial number: 12
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

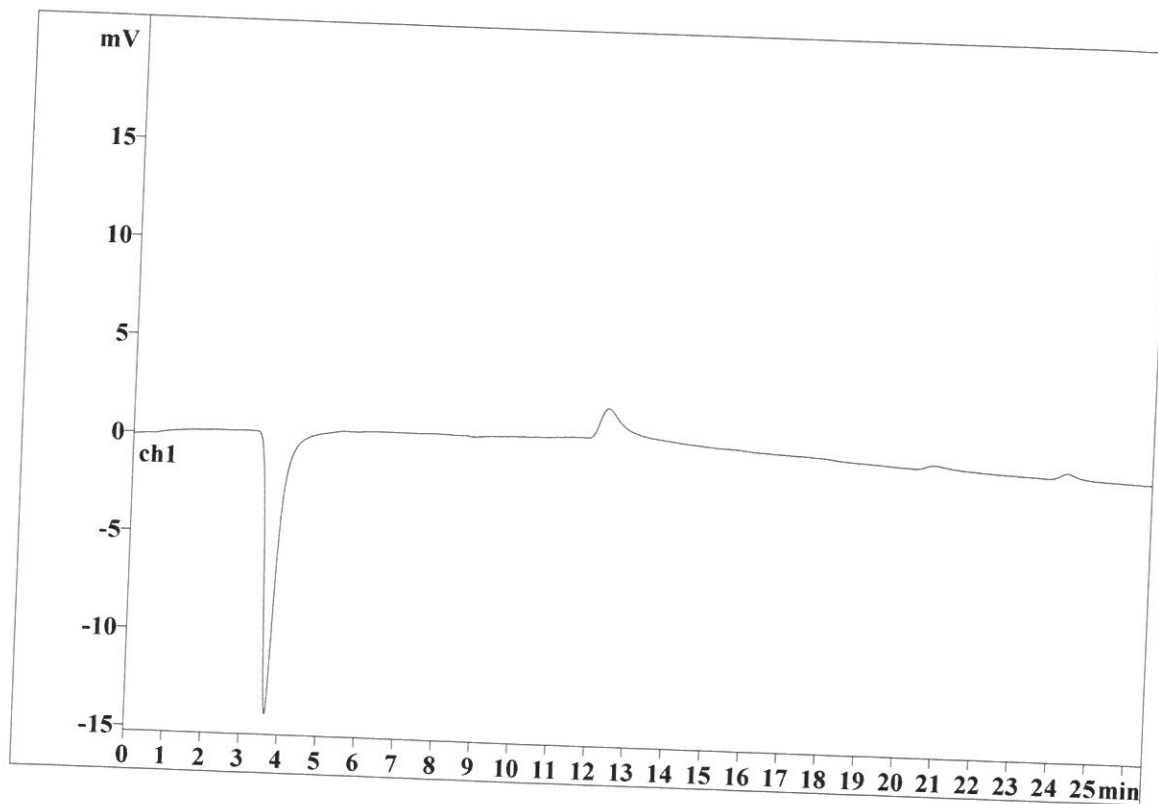

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD