


LB 117976

7470A

INSTRUMENT ID: CV1

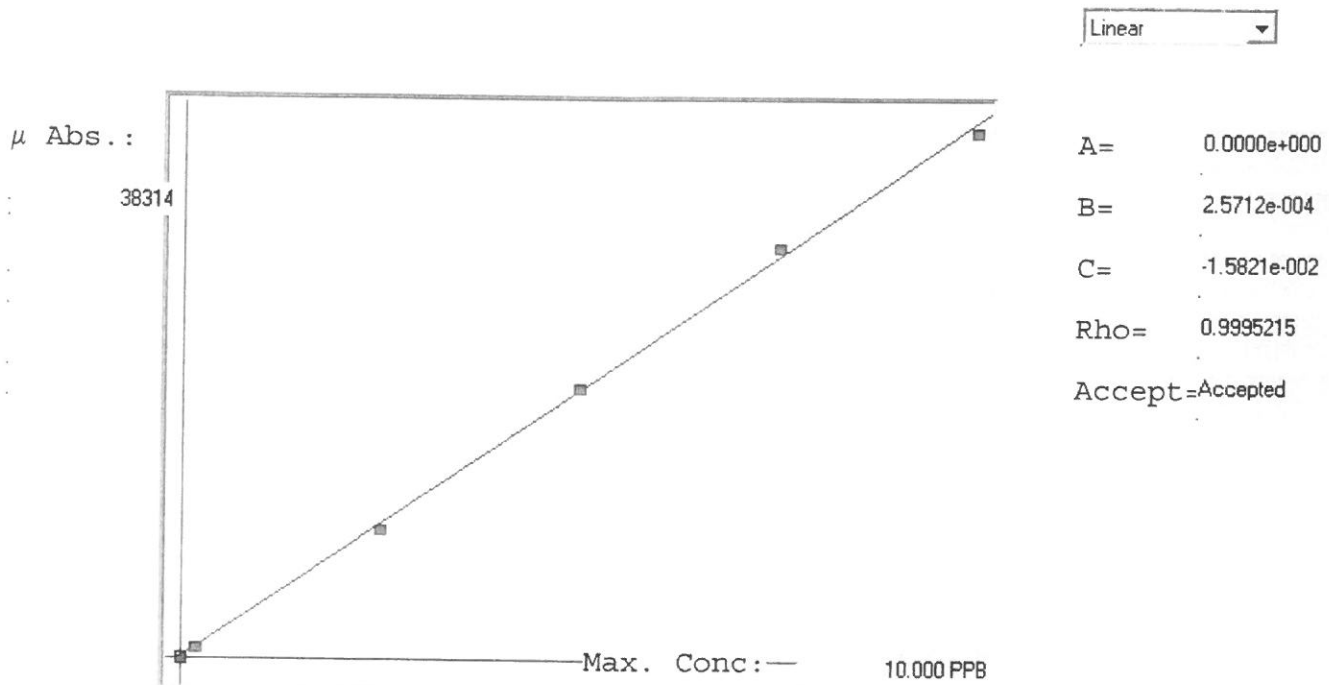

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	0.002	0.002	70	0.000	70					
0.2	0.200	0.192	-0.008	810	0.0 %	810					-4
2.5	2.500	2.407	-0.093	9421	0.0 %	9421					-4
5.0	5.000	5.069	0.069	19777	0.0 %	19777					1
7.5	7.500	7.694	0.194	29984	0.0 %	29984					3
10.0	10.000	9.836	-0.164	38314	0.0 %	38314					-2

LB117976 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 27 Dec 2021 12:08:43

Sample ID	Extended ID	μ Abs	Conc	Std ConcMethod	Units	Date	Type	Type
0.0 - 1	50	70	-	0.00007470A	PPB	27 Dec 2021 12:10:40	S	Std
0.2 - 1	50.2	810	-	0.20007470A	PPB	27 Dec 2021 12:12:57	S	Std
2.5 - 1	52.5	9421	-	2.50007470A	PPB	27 Dec 2021 12:15:14	S	Std
5.0 - 1	55	19777	-	5.00007470A	PPB	27 Dec 2021 12:17:31	S	Std
7.5 - 1	57.5	29984	-	7.50007470A	PPB	27 Dec 2021 12:19:47	S	Std
10.0 - 1	50	38314	-	10.00007470A	PPB	27 Dec 2021 12:24:35	S	Std
ICV25 - 1	ICV25	15412	3.9470	-7470A	PPB	27 Dec 2021 12:27:14	U	SMPL
ICB25 - 1	ICB25	-25	-0.0222	-7470A	PPB	27 Dec 2021 12:29:29	U	SMPL
CCV01 - 1	CCV01	19726	5.0562	-7470A	PPB	27 Dec 2021 12:31:43	U	SMPL
CCB01 - 1	CCB01	-27	-0.0228	-7470A	PPB	27 Dec 2021 12:33:59	U	SMPL
CRA - 1	CRA	762	0.1801	-7470A	PPB	27 Dec 2021 12:36:13	U	SMPL
HighStd - 1	HighStd	38022	9.7606	-7470A	PPB	27 Dec 2021 12:38:29	U	SMPL
ChkStd - 1	ChkStd	27744	7.1179	-7470A	PPB	27 Dec 2021 12:40:44	U	SMPL
PB141677BL - 1	PBW	32	-0.0076	-7470A	PPB	27 Dec 2021 12:43:01	U	SMPL
PB141677BS - 1	LCSW	15410	3.9465	-7470A	PPB	27 Dec 2021 12:45:17	U	SMPL
M5188-01 - 1	SASP2-119-1-COMP	126	0.0166	-7470A	PPB	27 Dec 2021 12:47:34	U	SMPL
M5208-02 - 1	WP-SOIL-1	143	0.0209	-7470A	PPB	27 Dec 2021 12:49:50	U	SMPL
M5208-02MS - 1	WP-SOIL-1MS	15328	3.9254	-7470A	PPB	27 Dec 2021 12:54:24	U	SMPL
M5208-02MSD - 1	WP-SOIL-1MSD	15126	3.8735	-7470A	PPB	27 Dec 2021 12:56:40	U	SMPL
CCV02 - 1	CCV02	19929	5.1084	-7470A	PPB	27 Dec 2021 12:58:55	U	SMPL
CCB02 - 1	CCB02	-24	-0.0220	-7470A	PPB	27 Dec 2021 13:01:11	U	SMPL
PB141678BL - 1	PBW	35	-0.0068	-7470A	PPB	27 Dec 2021 13:03:26	U	SMPL
PB141678BS - 1	LCSW	14635	3.7472	-7470A	PPB	27 Dec 2021 13:05:42	U	SMPL
M5219-02 - 1	M21013-N48854-1040	-19	-0.0207	-7470A	PPB	27 Dec 2021 13:07:57	U	SMPL
M5219-02DUP - 1	M21013-N48854-1040DUP	125	0.0163	-7470A	PPB	27 Dec 2021 13:10:13	U	SMPL
M5219-02MS - 1	M21013-N48854-1040MS	15364	3.9346	-7470A	PPB	27 Dec 2021 13:12:29	U	SMPL
M5219-02MSD - 1	M21013-N48854-1040MSD	14734	3.7727	-7470A	PPB	27 Dec 2021 13:14:45	U	SMPL
PB141679BL - 1	PBW	24	-0.0097	-7470A	PPB	27 Dec 2021 13:17:02	U	SMPL
PB141679BS - 1	LCSW	13718	3.5114	-7470A	PPB	27 Dec 2021 13:19:18	U	SMPL
M5219-01 - 1	M21013-N48854-1040	53	-0.0022	-7470A	PPB	27 Dec 2021 13:21:36	U	SMPL
M5219-01DUP - 1	M21013-N48854-1040DUP	53	-0.0022	-7470A	PPB	27 Dec 2021 13:23:52	U	SMPL
CCV03 - 1	CCV03	19604	5.0249	-7470A	PPB	27 Dec 2021 13:26:07	U	SMPL
CCB03 - 1	CCB03	-20	-0.0210	-7470A	PPB	27 Dec 2021 13:28:22	U	SMPL
M5219-01MS - 1	M21013-N48854-1040MS	14365	3.6778	-7470A	PPB	27 Dec 2021 13:30:38	U	SMPL
M5219-01MSD - 1	M21013-N48854-1040MSD	14637	3.7477	-7470A	PPB	27 Dec 2021 13:32:54	U	SMPL
M5208-02DUP - 1	WP-SOIL-1DUP	79	0.0045	-7470A	PPB	27 Dec 2021 13:35:10	U	SMPL
PB141677TB - 1	PB141639TB	83	0.0055	-7470A	PPB	27 Dec 2021 13:37:25	U	SMPL
PB141678TB - 1	PB141649TB	48	-0.0035	-7470A	PPB	27 Dec 2021 13:39:41	U	SMPL
M5208-02LX5 - 1		54	-0.0019	-7470A	PPB	27 Dec 2021 13:41:58	U	SMPL
M5208-02A - 1		15452	3.9573	-7470A	PPB	27 Dec 2021 13:44:14	U	SMPL
M5219-02LX5 - 1		-19	-0.0207	-7470A	PPB	27 Dec 2021 13:46:31	U	SMPL
M5219-02A - 1		15346	3.9300	-7470A	PPB	27 Dec 2021 13:48:48	U	SMPL
CCV04 - 1	CCV04	19557	5.0128	-7470A	PPB	27 Dec 2021 13:51:03	U	SMPL
CCB04 - 1	CCB04	-19	-0.0207	-7470A	PPB	27 Dec 2021 13:53:18	U	SMPL
M5219-01LX5 - 1		19	-0.0109	-7470A	PPB	27 Dec 2021 13:55:34	U	SMPL
M5219-01A - 1		15453	3.9575	-7470A	PPB	27 Dec 2021 13:57:50	U	SMPL
CCV05 - 1	CCV05	19674	5.0429	-7470A	PPB	27 Dec 2021 14:00:06	U	SMPL
CCB05 - 1	CCB05	-16	-0.0199	-7470A	PPB	27 Dec 2021 14:02:21	U	SMPL