

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12 Instrument ID : Konelab

12/29/2021 13:49

Test: Total CN

Sample Id	^{mp} Result	Dil. 1 +	Response	Errors
ICV1	98.257	0.0	0.084	
ICB1	0.973	0.0	0.001	
CCV1	241.952	0.0	0.206	
CCB1	0.677	0.0	0.001	
PB141749BL	0.671	0.0	0.001	
M5237-02	0.700	0.0	0.001	
M5237-02DUP	0.783	0.0	0.001	
M5237-05	1.572	0.0	0.002	
M5241-02	0.560	0.0	0.001	
M5241-05	0.494	0.0	0.001	
CCV2	255.265	0.0	0.218	
CCB2	0.566	0.0	0.001	

N	12
Mean	50.206
SD	96.8195
CV%	192.85

Aquakem v. 7.2AQ1

Results from time period:

Wed Dec 29 13:19:12 2021

Wed Dec 29 13:47:31 2021

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.0PPBCN	A	Total CN	P	-0.1614	µg/l	12/29/2021 13:19:12	
5.0PPBCN	A	Total CN	P	4.8235	µg/l	12/29/2021 13:19:13	
10PPBCN	A	Total CN	P	10.0085	µg/l	12/29/2021 13:19:14	
50PPBCN	A	Total CN	P	49.2561	µg/l	12/29/2021 13:19:15	
100PPBCN	A	Total CN	P	100.4335	µg/l	12/29/2021 13:19:16	
250PPBCN	A	Total CN	P	251.3012	µg/l	12/29/2021 13:19:17	
500PPBCN	A	Total CN	P	499.3387	µg/l	12/29/2021 13:19:18	
ICV1	S	Total CN	P	98.2566	µg/l	12/29/2021 13:42:40	
ICB1	S	Total CN	P	0.9726	µg/l	12/29/2021 13:42:43	
CCV1	S	Total CN	P	241.9522	µg/l	12/29/2021 13:42:45	
CCB1	S	Total CN	P	0.6769	µg/l	12/29/2021 13:42:47	
PB141749BL	S	Total CN	P	0.6715	µg/l	12/29/2021 13:42:48	
M5237-02	S	Total CN	P	0.7	µg/l	12/29/2021 13:42:49	
M5237-02DUP	S	Total CN	P	0.7832	µg/l	12/29/2021 13:42:50	
M5237-05	S	Total CN	P	1.5719	µg/l	12/29/2021 13:47:27	
M5241-02	S	Total CN	P	0.56	µg/l	12/29/2021 13:47:28	
M5241-05	S	Total CN	P	0.494	µg/l	12/29/2021 13:47:29	
CCV2	S	Total CN	P	255.2647	µg/l	12/29/2021 13:47:30	
CCB2	S	Total CN	P	0.5664	µg/l	12/29/2021 13:47:31	

CHEMTECH CONSULTING GROUP INC

284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12

Instrument ID : Konelab

12/29/2021 13:19


Test Total CN

Accepted 12/29/2021 13:19

Factor 1174
Bias 0

Coeff. of det. 0.999986

Errors

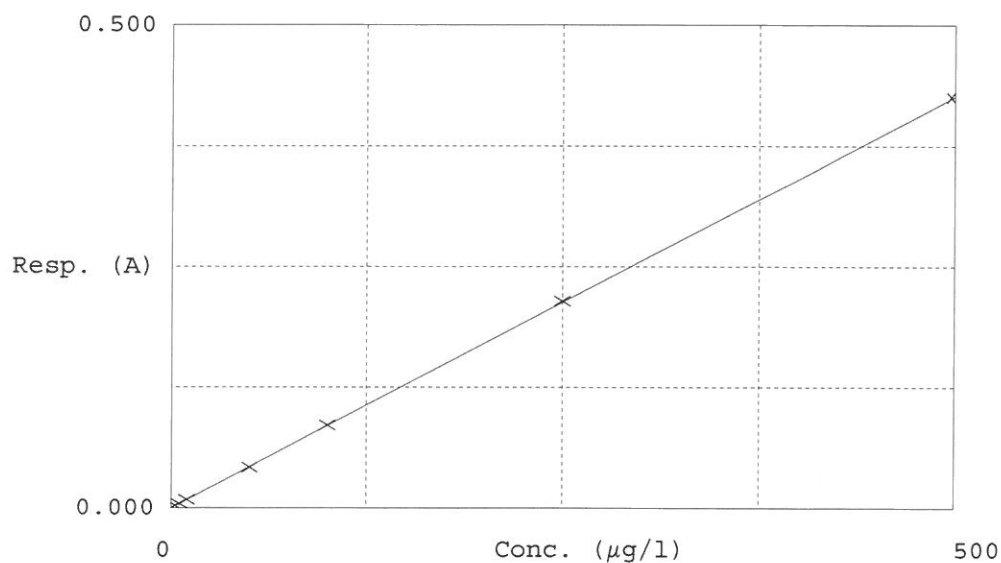

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.000	-0.1614	0.0000	-
2	5.0PPBCN	0.004	4.8235	5.0000	-3.5
3	10PPBCN	0.009	10.0085	10.0000	0.1
4	50PPBCN	0.042	49.2561	50.0000	-1.5
5	100PPBCN	0.086	100.4335	100.0000	0.4
6	250PPBCN	0.214	251.3012	250.0000	0.5
7	500PPBCN	0.426	499.3387	500.0000	-0.1

12 12/29/21