

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

12/29/2021 15:23

Reviewed by : 12 Instrument ID : Konelab

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	98.418	0.0	0.084	
ICB1	1.270	0.0	0.001	
CCV1	244.389	0.0	0.208	
CCB1	1.336	0.0	0.001	
PB141751BL	0.976	0.0	0.001	
PB141751BS	99.236	0.0	0.085	
LOWPB141751	10.594	0.0	0.009 - 105% (90-110)	
HIGHPB141751	491.256	0.0	0.419 - 98% (90-110)	
M5234-01	0.890	0.0	0.001	
M5234-01DUP	0.746	0.0	0.001	
M5234-01MS	32.074	0.0	0.028	
M5234-01MSD	31.916	0.0	0.027	
M5234-02	0.579	0.0	0.001	
CCV2	248.140	0.0	0.212	
CCB2	1.015	0.0	0.001	

N 15
Mean 84.189
SD 140.9195
CV% 167.38

12 12/29/21

Aquakem v. 7.2AQ1

Results from time period:

Wed Dec 29 15:15:39 2021

Wed Dec 29 15:22:26 2021

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Total CN	P	-0.1614	µg/l	12/29/2021 13:19:12	
5.OPPBCN	A	Total CN	P	4.8235	µg/l	12/29/2021 13:19:13	
10PPBCN	A	Total CN	P	10.0085	µg/l	12/29/2021 13:19:14	
50PPBCN	A	Total CN	P	49.2561	µg/l	12/29/2021 13:19:15	
100PPBCN	A	Total CN	P	100.4335	µg/l	12/29/2021 13:19:16	
250PPBCN	A	Total CN	P	251.3012	µg/l	12/29/2021 13:19:17	
500PPBCN	A	Total CN	P	499.3387	µg/l	12/29/2021 13:19:18	
ICV1	S	Total CN	P	98.4178	µg/l	12/29/2021 15:15:40	
ICB1	S	Total CN	P	1.2701	µg/l	12/29/2021 15:15:42	
CCV1	S	Total CN	P	244.3888	µg/l	12/29/2021 15:15:44	
CCB1	S	Total CN	P	1.3356	µg/l	12/29/2021 15:15:46	
PB141751BL	S	Total CN	P	0.9755	µg/l	12/29/2021 15:15:47	
PB141751BS	S	Total CN	P	99.2359	µg/l	12/29/2021 15:15:48	
LOWPB141751	S	Total CN	P	10.5936	µg/l	12/29/2021 15:22:18	
HIGHPB141751	S	Total CN	P	491.2563	µg/l	12/29/2021 15:22:19	
M5234-01	S	Total CN	P	0.8902	µg/l	12/29/2021 15:22:20	
M5234-01DUP	S	Total CN	P	0.7458	µg/l	12/29/2021 15:22:21	
M5234-01MS	S	Total CN	P	32.0736	µg/l	12/29/2021 15:22:22	
M5234-01MSD	S	Total CN	P	31.9155	µg/l	12/29/2021 15:22:23	
M5234-02	S	Total CN	P	0.5787	µg/l	12/29/2021 15:22:24	
CCV2	S	Total CN	P	248.1403	µg/l	12/29/2021 15:22:25	
CCB2	S	Total CN	P	1.0151	µg/l	12/29/2021 15:22:26	

CHEMTECH CONSULTING GROUP INC

284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12

Instrument ID : Konelab

12/29/2021 13:19

Test Total CN


Accepted 12/29/2021 13:19

Factor 1174

Bias 0

Coeff. of det. 0.999986

Errors

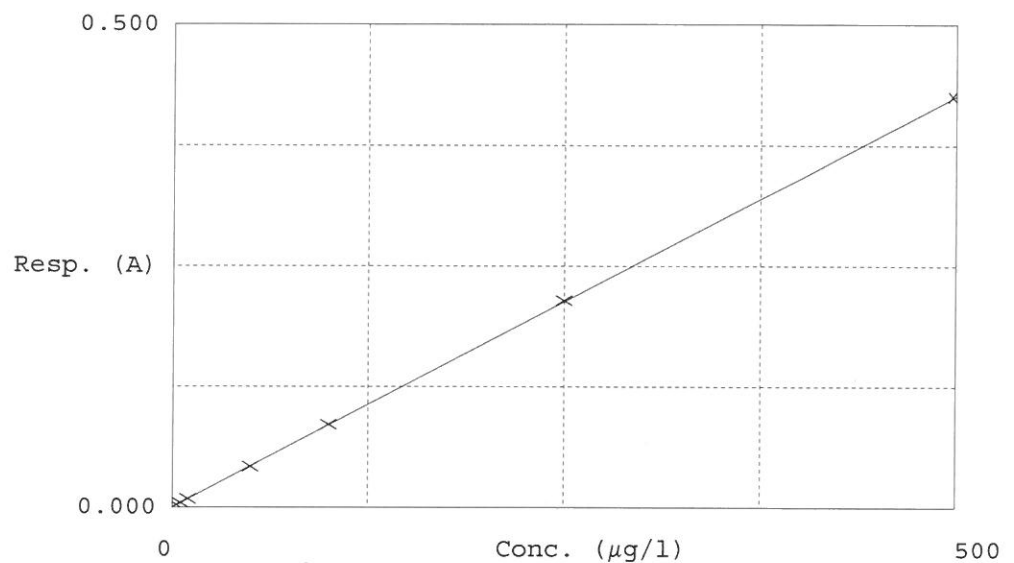

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.000	-0.1614	0.0000	-
2	5.0PPBCN	0.004	4.8235	5.0000	-3.5
3	10PPBCN	0.009	10.0085	10.0000	0.1
4	50PPBCN	0.042	49.2561	50.0000	-1.5
5	100PPBCN	0.086	100.4335	100.0000	0.4
6	250PPBCN	0.214	251.3012	250.0000	0.5
7	500PPBCN	0.426	499.3387	500.0000	-0.1

12 12/29/21