


LB118026

7471B

INSTRUMENT ID: CV1

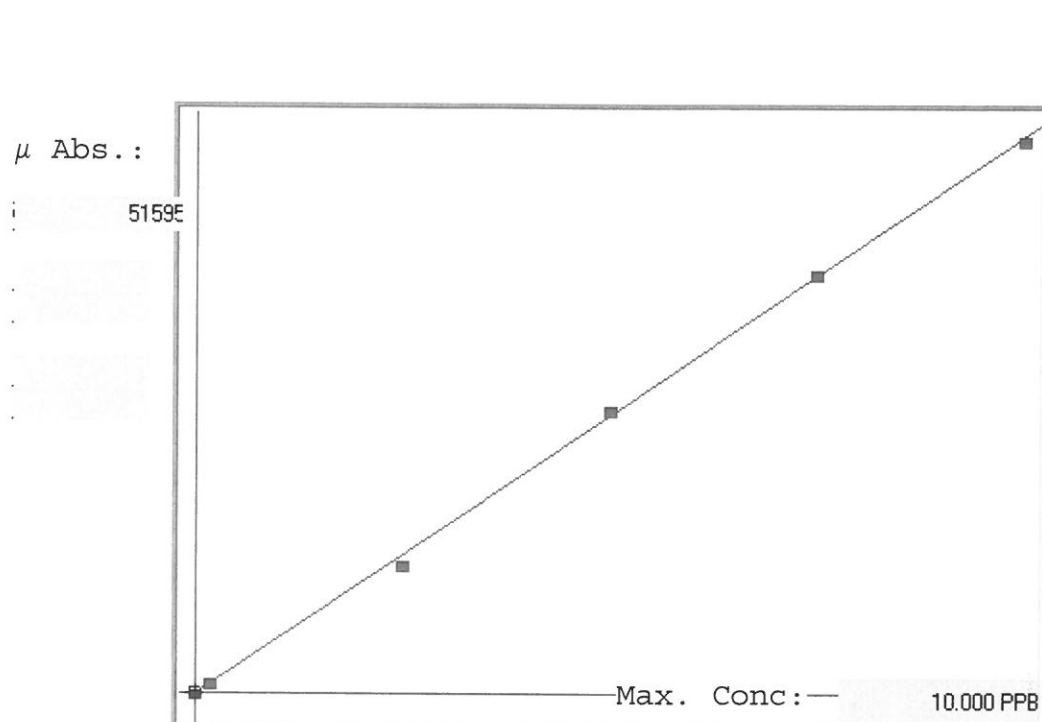

A= 0.0000e+000

B= 1.9209e-004

C= 1.9854e-002

Rho= 0.9997005

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	0.029	0.029	50	0.000	50					-
0.2	0.200	0.220	0.020	1043	0.0 %	1043					10
2.5	2.500	2.342	-0.158	12087	0.0 %	12087					-6
5.0	5.000	5.120	0.120	26549	0.0 %	26549					2
7.5	7.500	7.559	0.059	39247	0.0 %	39247					1
10.0	10.000	9.931	-0.069	51595	0.0 %	51595					-1

LB118026 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 30 Dec 2021 13:40:20

Sample ID	Extended ID	μ Abs	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	50	-	0.0000	7471B	PPB	30 Dec 2021 13:42:04	S	Std
0.2 - 1	50.2	1043	-	0.2000	7471B	PPB	30 Dec 2021 13:47:00	S	Std
2.5 - 1	52.5	12087	-	2.5000	7471B	PPB	30 Dec 2021 13:49:17	S	Std
5.0 - 1	55	26549	-	5.0000	7471B	PPB	30 Dec 2021 13:54:05	S	Std
7.5 - 1	59.5	39247	-	7.5000	7471B	PPB	30 Dec 2021 13:56:22	S	Std
10.0 - 1	518	51595	-	10.0000	7471B	PPB	30 Dec 2021 13:58:38	S	Std
ICV29 - 1	ICV29	20920	4.0383	-	7471B	PPB	30 Dec 2021 14:01:18	U	SMPL
ICB29 - 1	ICB29	-16	0.0168	-	7471B	PPB	30 Dec 2021 14:03:32	U	SMPL
CCV30 - 1	CCV30	27074	5.2204	-	7471B	PPB	30 Dec 2021 14:05:48	U	SMPL
CCB30 - 1	CCB30	-25	0.0151	-	7471B	PPB	30 Dec 2021 14:08:03	U	SMPL
CRA - 1	CRA	1038	0.2192	-	7471B	PPB	30 Dec 2021 14:10:18	U	SMPL
HighStd - 1	HighStd	52884	10.1781	-	7471B	PPB	30 Dec 2021 14:12:33	U	SMPL
ChkStd - 1	ChkStd	35764	6.8896	-	7471B	PPB	30 Dec 2021 14:14:49	U	SMPL
PB141775BL - 1	PBS	-46	0.0110	-	7471B	PPB	30 Dec 2021 14:17:06	U	SMPL
PB141775BS - 1	LCSS	19249	3.7173	-	7471B	PPB	30 Dec 2021 14:19:22	U	SMPL
M5196-23 - 1	COMPOSITE-SAMPLE-1-SHALLOW	421	0.1007	-	7471B	PPB	30 Dec 2021 14:21:38	U	SMPL
M5196-24 - 1	COMPOSITE-SAMPLE-1-DEEP	775	0.1687	-	7471B	PPB	30 Dec 2021 14:23:55	U	SMPL
M5196-25 - 1	COMPOSITE-SAMPLE-2-SHALLOW	1072	0.2258	-	7471B	PPB	30 Dec 2021 14:26:12	U	SMPL
M5196-26 - 1	COMPOSITE-SAMPLE-2-DEEP	532	0.1220	-	7471B	PPB	30 Dec 2021 14:28:30	U	SMPL
M5196-27 - 1	COMPOSITE-SAMPLE-3-SHALLOW	607	0.1365	-	7471B	PPB	30 Dec 2021 14:30:46	U	SMPL
CCV31 - 1	CCV31	27164	5.2377	-	7471B	PPB	30 Dec 2021 14:33:01	U	SMPL
CCB31 - 1	CCB31	-32	0.0137	-	7471B	PPB	30 Dec 2021 14:35:16	U	SMPL
M5196-28 - 1	COMPOSITE-SAMPLE-3-DEEP	746	0.1632	-	7471B	PPB	30 Dec 2021 14:37:31	U	SMPL
M5196-29 - 1	COMPOSITE-SAMPLE-4-SHALLOW	437	0.1038	-	7471B	PPB	30 Dec 2021 14:39:47	U	SMPL
M5196-30 - 1	COMPOSITE-SAMPLE-4-DEEP	485	0.1130	-	7471B	PPB	30 Dec 2021 14:42:02	U	SMPL
M5196-31 - 1	COMPOSITE-SAMPLE-5-SHALLOW	411	0.0988	-	7471B	PPB	30 Dec 2021 14:44:17	U	SMPL
M5196-31DUP - 1	COMPOSITE-SAMPLE-5-SHALLOWDUP	403	0.0973	-	7471B	PPB	30 Dec 2021 14:46:33	U	SMPL
M5196-31MS - 1	COMPOSITE-SAMPLE-5-SHALLOWMS	19459	3.7577	-	7471B	PPB	30 Dec 2021 14:48:49	U	SMPL
M5196-31MSD - 1	COMPOSITE-SAMPLE-5-SHALLOWMSD	20679	3.9920	-	7471B	PPB	30 Dec 2021 14:51:06	U	SMPL
M5241-01 - 1	TP-2S	3102	0.6157	-	7471B	PPB	30 Dec 2021 14:53:22	U	SMPL
M5241-04 - 1	TP-2D	8293	1.6128	-	7471B	PPB	30 Dec 2021 14:55:39	U	SMPL
M5245-01 - 1	SASP2-123-1-65-72	1156	0.2419	-	7471B	PPB	30 Dec 2021 14:57:55	U	SMPL
CCV32 - 1	CCV32	27312	5.2661	-	7471B	PPB	30 Dec 2021 15:00:10	U	SMPL
CCB32 - 1	CCB32	-4	0.0191	-	7471B	PPB	30 Dec 2021 15:02:26	U	SMPL
M5253-01 - 1	SA-1-122921	1638	0.3345	-	7471B	PPB	30 Dec 2021 15:04:43	U	SMPL
M5254-01 - 1	361	1590	0.3253	-	7471B	PPB	30 Dec 2021 15:06:59	U	SMPL
M5255-01 - 1	TR-04-122921	2741	0.5464	-	7471B	PPB	30 Dec 2021 15:09:14	U	SMPL
M5256-01 - 1	BU-03-122921	978	0.2077	-	7471B	PPB	30 Dec 2021 15:11:30	U	SMPL
M5257-01 - 1	D3-12292021	161206	30.9853	-	7471B	PPB	30 Dec 2021 15:13:46	U	SMPL
M5196-31LX5 - 1		-144	-0.0078	-	7471B	PPB	30 Dec 2021 15:16:02	U	SMPL
M5196-31A - 1		21332	4.1174	-	7471B	PPB	30 Dec 2021 15:18:21	U	SMPL
M5257-01DLX5 - 1		33012	6.3610	-	7471B	PPB	30 Dec 2021 15:28:32	U	SMPL
CCV33 - 1	CCV33	25950	5.0045	-	7471B	PPB	30 Dec 2021 15:39:25	U	SMPL
CCB33 - 1	CCB33	-64	0.0076	-	7471B	PPB	30 Dec 2021 15:41:41	U	SMPL