


LB118071

7470A

INSTRUMENT ID: 101

Linear

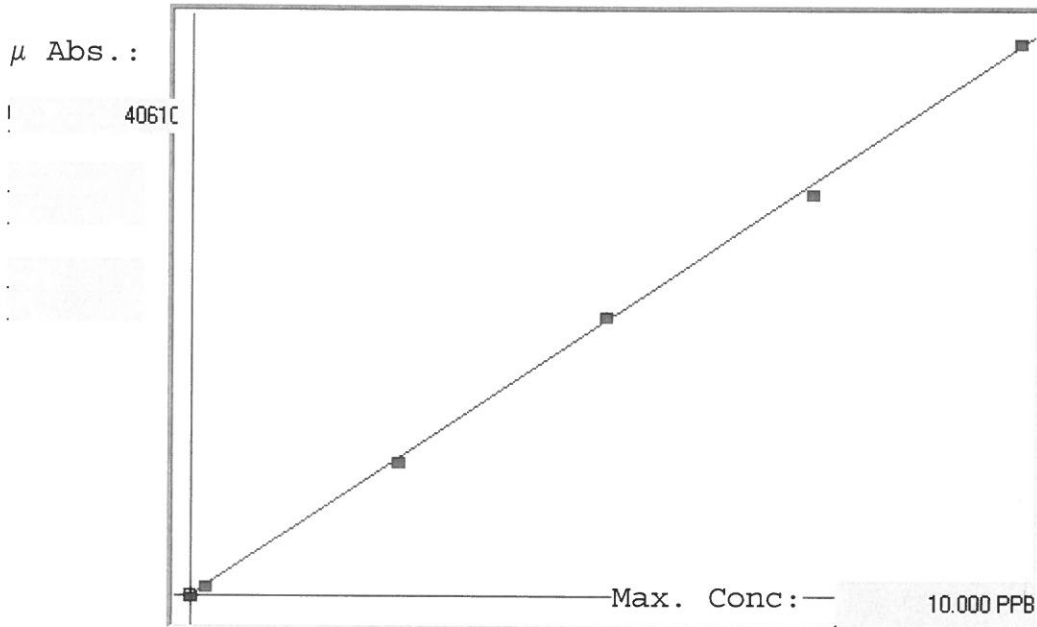

A= 0.0000e+000

B= 2.4780e-004

C= 8.7179e-003

Rho= 0.9996912

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%))
0.0	0.000	0.026	0.026	70	0.000	70					5
0.2	0.200	0.193	-0.007	743	0.0 %	743					-4
2.5	2.500	2.457	-0.043	9881	0.0 %	9881					-2
5.0	5.000	5.120	0.120	20628	0.0 %	20628					2
7.5	7.500	7.332	-0.168	29553	0.0 %	29553					-2
10.0	10.000	10.072	0.072	40610	0.0 %	40610					1

LB118071 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 05 Jan 2022 12:47:16

Sample ID	Extended ID	μ Abs	Conc	Std CondMethod	Units	Date	Type	Type
0.0 - 1	50	70	-	0.00007470A	PPB	05 Jan 2022 13:19:21	S	Std
0.2 - 1	50.2	743	-	0.20007470A	PPB	05 Jan 2022 13:21:39	S	Std
2.5 - 1	52.5	9881	-	2.50007470A	PPB	05 Jan 2022 13:23:56	S	Std
5.0 - 1	55	20628	-	5.00007470A	PPB	05 Jan 2022 13:26:13	S	Std
7.5 - 1	57.5	29553	-	7.50007470A	PPB	05 Jan 2022 13:31:01	S	Std
10.0 - 1	510	40610	-	10.00007470A	PPB	05 Jan 2022 13:33:16	S	Std
ICV33 - 1	ICV33	14672	3.6444	-7470A	PPB	05 Jan 2022 13:35:57	U	SMPL
ICB33 - 1	ICB33	20	0.0137	-7470A	PPB	05 Jan 2022 13:38:12	U	SMPL
CCV44 - 1	CCV44	19585	4.8618	-7470A	PPB	05 Jan 2022 13:40:27	U	SMPL
CCB44 - 1	CCB44	14	0.0122	-7470A	PPB	05 Jan 2022 13:42:42	U	SMPL
CRA - 1	CRA	748	0.1941	-7470A	PPB	05 Jan 2022 13:44:57	U	SMPL
HighStd - 1	HighStd	40362	10.0103	-7470A	PPB	05 Jan 2022 13:47:12	U	SMPL
ChkStd - 1	ChkStd	29006	7.1963	-7470A	PPB	05 Jan 2022 13:49:28	U	SMPL
PB141853BL - 1	PBW	97	0.0328	-7470A	PPB	05 Jan 2022 13:51:44	U	SMPL
PB141853BS - 1	LCSW	13540	3.3639	-7470A	PPB	05 Jan 2022 13:54:00	U	SMPL
N1002-02 - 1	BLACK-DRUM	227	0.0650	-7470A	PPB	05 Jan 2022 14:05:37	U	SMPL
N1002-04 - 1	BLUE-DRUM	240	0.0682	-7470A	PPB	05 Jan 2022 14:07:53	U	SMPL
N1007-03 - 1	BARNUM-ST-SP	207	0.0600	-7470A	PPB	05 Jan 2022 14:10:10	U	SMPL
N1014-02 - 1	72-11944	178	0.0528	-7470A	PPB	05 Jan 2022 14:12:28	U	SMPL
N1016-02 - 1	E3	235	0.0670	-7470A	PPB	05 Jan 2022 14:14:43	U	SMPL
CCV45 - 1	CCV45	19977	4.9590	-7470A	PPB	05 Jan 2022 14:16:59	U	SMPL
CCB45 - 1	CCB45	15	0.0124	-7470A	PPB	05 Jan 2022 14:19:14	U	SMPL
N1016-02DUP - 1	E3DUP	116	0.0375	-7470A	PPB	05 Jan 2022 14:21:30	U	SMPL
N1016-02MS - 1	E3MS	14450	3.5894	-7470A	PPB	05 Jan 2022 14:23:46	U	SMPL
N1016-02MSD - 1	E3MSD	13628	3.3857	-7470A	PPB	05 Jan 2022 14:26:01	U	SMPL
PB141854BL - 1	PBW	23	0.0144	-7470A	PPB	05 Jan 2022 14:28:17	U	SMPL
PB141854BS - 1	LCSW	14268	3.5443	-7470A	PPB	05 Jan 2022 14:33:07	U	SMPL
N1010-01 - 1	20211307-CAPE-1-SITE-WATER	81	0.0288	-7470A	PPB	05 Jan 2022 14:35:23	U	SMPL
N1010-01DUP - 1	20211307-CAPE-1-SITE-WATERDUP	79	0.0283	-7470A	PPB	05 Jan 2022 14:37:40	U	SMPL
N1010-01MS - 1	20211307-CAPE-1-SITE-WATERMS	15303	3.8008	-7470A	PPB	05 Jan 2022 14:39:57	U	SMPL
N1010-01MSD - 1	20211307-CAPE-1-SITE-WATERMSD	16168	4.0151	-7470A	PPB	05 Jan 2022 14:42:14	U	SMPL
N1010-02 - 1	20211308-CAPE-2-SITE-WATER	88	0.0305	-7470A	PPB	05 Jan 2022 14:44:30	U	SMPL
CCV46 - 1	CCV46	20255	5.0278	-7470A	PPB	05 Jan 2022 14:46:45	U	SMPL
CCB46 - 1	CCB46	-5	0.0075	-7470A	PPB	05 Jan 2022 14:49:01	U	SMPL
N1010-03 - 1	20211309-CAPE-3-SITE-WATER	106	0.0350	-7470A	PPB	05 Jan 2022 14:51:16	U	SMPL
N1010-04 - 1	20211310-CAPE-4-SITE-WATER	107	0.0352	-7470A	PPB	05 Jan 2022 14:53:32	U	SMPL
N1010-05 - 1	20211311-CAPE-5-SITE-WATER	100	0.0335	-7470A	PPB	05 Jan 2022 14:55:48	U	SMPL
N1010-06 - 1	20211312-CAPE-6-SITE-WATER	96	0.0323	-7470A	PPB	05 Jan 2022 14:58:04	U	SMPL
N1010-07 - 1	20211306-FIELD-BLANK	29	0.0159	-7470A	PPB	05 Jan 2022 15:00:20	U	SMPL
N1012-21 - 1	COMP-31332:34	10355	2.5747	-7470A	PPB	05 Jan 2022 15:02:36	U	SMPL
N1018-09 - 1	FB-010422	243	0.0689	-7470A	PPB	05 Jan 2022 15:04:53	U	SMPL
CCV47 - 1	CCV47	20018	4.9691	-7470A	PPB	05 Jan 2022 15:07:10	U	SMPL
CCB47 - 1	CCB47	-35	0.0000	-7470A	PPB	05 Jan 2022 15:09:26	U	SMPL
PB141830TB - 1	PB141830TB	220	0.0632	-7470A	PPB	05 Jan 2022 15:11:42	U	SMPL
N1016-02LX5 - 1		48	0.0206	-7470A	PPB	05 Jan 2022 15:13:58	U	SMPL
N1016-02A - 1		15510	3.8521	-7470A	PPB	05 Jan 2022 15:16:13	U	SMPL
N1010-01LX5 - 1		-22	0.0033	-7470A	PPB	05 Jan 2022 15:18:29	U	SMPL
N1010-01A - 1		15840	3.9338	-7470A	PPB	05 Jan 2022 15:20:45	U	SMPL
CCV48 - 1	CCV48	20129	4.9966	-7470A	PPB	05 Jan 2022 15:23:00	U	SMPL
CCB48 - 1	CCB48	-22	0.0033	-7470A	PPB	05 Jan 2022 15:25:16	U	SMPL