

LB118091

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092Reviewed by : 12 Instrument ID : Konelab

1/6/2022 11:51

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	95.961	0.0	0.077	
ICB1	0.549	0.0	0.001	
CCV1	247.037	0.0	0.197	
CCB1	0.754	0.0	0.001	
PB141879BL	0.566	0.0	0.001	
N1014-02	0.610	0.0	0.001	
N1016-02	0.498	0.0	0.001	
N1023-01	0.661	0.0	0.001	
N1007-03	0.238	0.0	0.001	
N1007-03DUP	0.411	0.0	0.001	
CCV2	260.068	0.0	0.207	
CCB2	0.301	0.0	0.001	

N	12
Mean	50.638
SD	98.6746
CV%	194.86

Aquakem v. 7.2AQ1

Results from time period:

Thu Jan 06 10:31:16 2022

Thu Jan 06 11:46:56 2022

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Total CN	P	0.2753	µg/l	1/6/2022 10:31:16	
5.OPPBCN	A	Total CN	P	5.0365	µg/l	1/6/2022 10:31:17	
10PPBCN	A	Total CN	P	9.9644	µg/l	1/6/2022 10:31:18	
50PPBCN	A	Total CN	P	49.1751	µg/l	1/6/2022 10:31:19	
100PPBCN	A	Total CN	P	99.0937	µg/l	1/6/2022 10:31:20	
250PPBCN	A	Total CN	P	252.382	µg/l	1/6/2022 10:31:21	
500PPBCN	A	Total CN	P	499.0732	µg/l	1/6/2022 10:31:22	
ICV1	S	Total CN	P	95.9608	µg/l	1/6/2022 11:17:37	
ICB1	S	Total CN	P	0.5494	µg/l	1/6/2022 11:17:38	
CCV1	S	Total CN	P	247.0369	µg/l	1/6/2022 11:17:41	
CCB1	S	Total CN	P	0.754	µg/l	1/6/2022 11:17:42	
PB141879BL	S	Total CN	P	0.5657	µg/l	1/6/2022 11:17:44	
N1014-02	S	Total CN	P	0.6105	µg/l	1/6/2022 11:17:45	
N1016-02	S	Total CN	P	0.4978	µg/l	1/6/2022 11:17:46	
N1023-01	S	Total CN	P	0.6613	µg/l	1/6/2022 11:22:23	
N1007-03	S	Total CN	P	0.2381	µg/l	1/6/2022 11:46:53	
N1007-03DUP	S	Total CN	P	0.4111	µg/l	1/6/2022 11:46:54	
CCV2	S	Total CN	P	260.0684	µg/l	1/6/2022 11:46:55	
CCB2	S	Total CN	P	0.301	µg/l	1/6/2022 11:46:56	

CHEMTECH CONSULTING GROUP INC
 284 Sheffield Street, Mountainside, NJ 07092

1/6/2022 10:38

Reviewed by : 12 Instrument ID : Konelab


Test Total CN

Accepted 1/6/2022 10:38

Factor 1257
 Bias 0

Coeff. of det. 0.999961

Errors

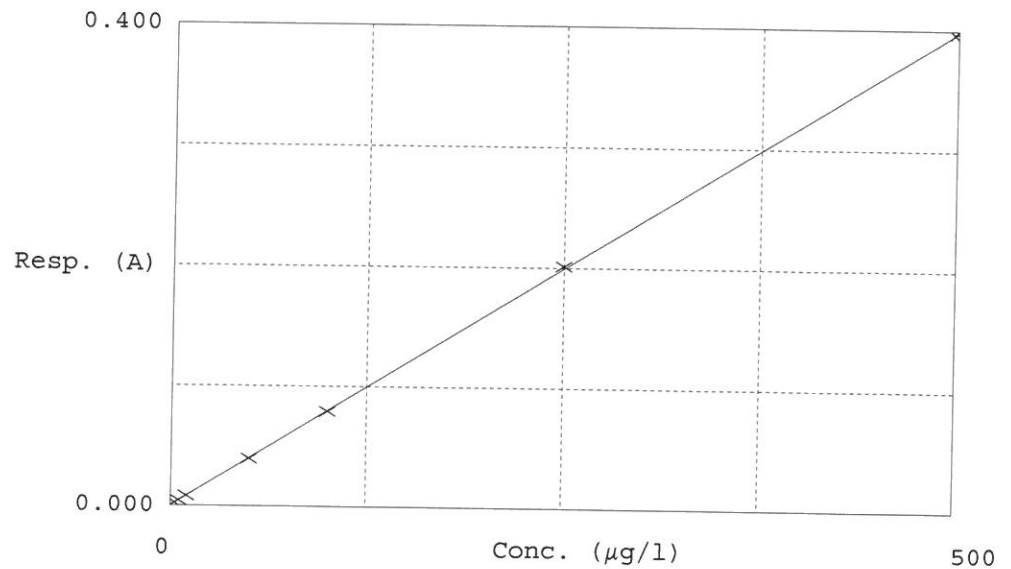

	Calibrator	Response	Calc. con.	Conc.	^{Re} Errors
1	0.0PPBCN	0.001	0.2753	0.0000	-
2	5.0PPBCN	0.004	5.0365	5.0000	0.7
3	10PPBCN	0.008	9.9644	10.0000	-0.4
4	50PPBCN	0.040	49.1751	50.0000	-1.6
5	100PPBCN	0.079	99.0937	100.0000	-0.9
6	250PPBCN	0.201	252.3820	250.0000	1.0
7	500PPBCN	0.398	499.0732	500.0000	-0.2

12 01/06/22