

=====

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

1/6/2022 16:28

Reviewed by : 12 Instrument ID : Konelab

Test: Total CN

Sample Id	<i>mp/12</i> Result	Dil. 1 +	Response	Errors
ICV1	94.996	0.0	0.076	
ICB1	0.563	0.0	0.001	
CCV1	245.616	0.0	0.196	
CCB1	0.646	0.0	0.001	
PB141847BL	0.729	0.0	0.001	
PB141847BS	246.779	0.0	0.197	
N1018-09	0.890	0.0	0.001	
N1041-01	1.101	0.0	0.001	
N1041-01DUP	1.182	0.0	0.001	
N1041-01MS	41.552	0.0	0.033	
N1041-01MSD	41.643	0.0	0.034	
N1047-05	0.678	0.0	0.001	
CCV2	249.029	0.0	0.199	
CCB2	1.002	0.0	0.001	

N	14
Mean	66.172
SD	101.6902
CV%	153.68

Aquakem v. 7.2AQ1

Results from time period:

Thu Jan 06 15:57:36 2022

Thu Jan 06 16:04:23 2022

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Total CN	P	0.2753	µg/l	1/6/2022 10:31:16	
5.OPPBCN	A	Total CN	P	5.0365	µg/l	1/6/2022 10:31:17	
10PPBCN	A	Total CN	P	9.9644	µg/l	1/6/2022 10:31:18	
50PPBCN	A	Total CN	P	49.1751	µg/l	1/6/2022 10:31:19	
100PPBCN	A	Total CN	P	99.0937	µg/l	1/6/2022 10:31:20	
250PPBCN	A	Total CN	P	252.382	µg/l	1/6/2022 10:31:21	
500PPBCN	A	Total CN	P	499.0732	µg/l	1/6/2022 10:31:22	
ICV1	S	Total CN	P	94.9958	µg/l	1/6/2022 15:57:37	
ICB1	S	Total CN	P	0.5626	µg/l	1/6/2022 15:57:38	
CCV1	S	Total CN	P	245.6156	µg/l	1/6/2022 15:57:41	
CCB1	S	Total CN	P	0.6462	µg/l	1/6/2022 15:57:43	
PB141847BL	S	Total CN	P	0.729	µg/l	1/6/2022 15:57:44	
PB141847BS	S	Total CN	P	246.7792	µg/l	1/6/2022 15:57:45	
N1018-09	S	Total CN	P	0.8903	µg/l	1/6/2022 15:57:46	
N1041-01	S	Total CN	P	1.1006	µg/l	1/6/2022 16:04:15	
N1041-01DUP	S	Total CN	P	1.1819	µg/l	1/6/2022 16:04:16	
N1041-01MS	S	Total CN	P	41.5521	µg/l	1/6/2022 16:04:19	
N1041-01MSD	S	Total CN	P	41.6427	µg/l	1/6/2022 16:04:20	
N1047-05	S	Total CN	P	0.6777	µg/l	1/6/2022 16:04:21	
CCV2	S	Total CN	P	249.0293	µg/l	1/6/2022 16:04:22	
CCB2	S	Total CN	P	1.002	µg/l	1/6/2022 16:04:23	

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12 Instrument ID : Konelab

1/6/2022 10:38


Test Total CN

Accepted 1/6/2022 10:38

Factor 1257
Bias 0

Coeff. of det. 0.999961

Errors

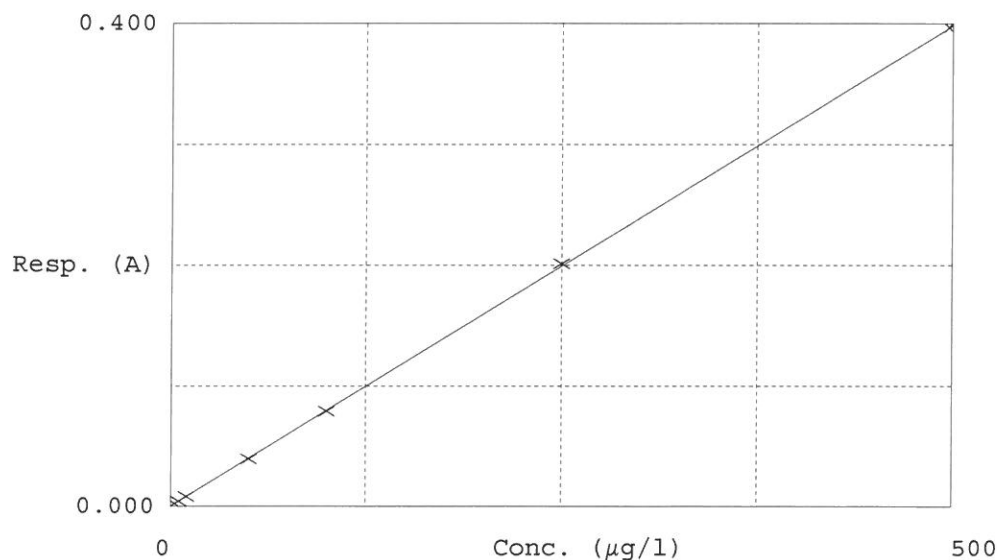

	Calibrator	Response	Calc. con.	Conc.	Re Errors
1	0.0PPBCN	0.001	0.2753	0.0000	-
2	5.0PPBCN	0.004	5.0365	5.0000	0.7
3	10PPBCN	0.008	9.9644	10.0000	-0.4
4	50PPBCN	0.040	49.1751	50.0000	-1.6
5	100PPBCN	0.079	99.0937	100.0000	-0.9
6	250PPBCN	0.201	252.3820	250.0000	1.0
7	500PPBCN	0.398	499.0732	500.0000	-0.2

12 01/06/22