

LB118189

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12

Instrument ID : Konelab

1/12/2022 11:17

Test: CNEPA-NEW

Sample Id	Result	Dil. 1 +	Response	Errors
ICV001 ICV001	93.508	0.0	0.097	
ICB001 ICB001	0.960	0.0	0.009	
CCV001 CCV001	251.274	0.0	0.248	
CCB001 CCB001	1.380	0.0	0.009	
PB141965BL PBS965	1.647	0.0	0.009	
N1030-01 EW2X0	1.110	0.0	0.009	
N1030-02 EW2W3	1.305	0.0	0.009	
N1030-03 EW2W7	1.662	0.0	0.009	
N1030-04 EW2W7D	1.534	0.0	0.009	
N1030-05 EW2W7S	96.798	0.0	0.100	
N1030-06 EW2Y1	0.910	0.0	0.009	
N1030-07 EW2W8	1.893	0.0	0.010	
N1030-08 EW2W9	1.215	0.0	0.009	
N1030-09 EW2X1	2.009	0.0	0.010	
N1030-10 EW2X3	2.810	0.0	0.011	
PB141966BL PBW966	1.684	0.0	0.010	
N1075-01 EW2W6	1.028	0.0	0.009	
N1075-02 EW310	0.733	0.0	0.009	
N1075-03 EW315	1.903	0.0	0.010	
N1075-04 EW315D	1.842	0.0	0.010	
N1075-05 EW315S	96.459	0.0	0.100	
N1075-06 EW318	2.168	0.0	0.010	
N1075-07 EW319	1.253	0.0	0.009	
N1075-08 EW321	2.942	0.0	0.011	
N1075-09 EW316	1.618	0.0	0.009	
N1075-10 EW317	1.195	0.0	0.009	
CCV002 CV002 CCV002	245.107	0.0	0.242	
CCB002 CCB002	0.777	0.0	0.009	

12
01/25/22

N	28
Mean	29.240
SD	68.5179
CV%	234.33

Aquakem v. 7.2AQ1

Results from time period:

Wed Jan 12 09:46:24 2022

Wed Jan 12 11:00:24 2022

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time
S0.0	A	CNEPA-NE\ P		0.5839	µg/l	1/12/2022 10:04:08
S5.0	A	CNEPA-NE\ P		4.7975	µg/l	1/12/2022 10:04:09
S10.0	A	CNEPA-NE\ P		10.2529	µg/l	1/12/2022 10:04:10
S100.0	A	CNEPA-NE\ P		100.0789	µg/l	1/12/2022 10:04:11
S250.0	A	CNEPA-NE\ P		248.6111	µg/l	1/12/2022 10:04:12
S500.0	A	CNEPA-NE\ P		500.6756	µg/l	1/12/2022 10:04:13
ICV001 ICV001	S	CNEPA-NE\ P		93.5079	µg/l	1/12/2022 10:41:53
ICB001 ICB001	S	CNEPA-NE\ P		0.96	µg/l	1/12/2022 10:41:54
CCV001 CCV001	S	CNEPA-NE\ P		251.2743	µg/l	1/12/2022 10:41:57
CCB001 CCB001	S	CNEPA-NE\ P		1.3797	µg/l	1/12/2022 10:41:58
PB141965BL PBS965	S	CNEPA-NE\ P		1.647	µg/l	1/12/2022 10:42:00
N1030-01 EW2X0	S	CNEPA-NE\ P		1.1098	µg/l	1/12/2022 10:42:01
N1030-02 EW2W3	S	CNEPA-NE\ P		1.3053	µg/l	1/12/2022 10:42:02
N1030-03 EW2W7	S	CNEPA-NE\ P		1.6617	µg/l	1/12/2022 10:49:25
N1030-04 EW2W7D	S	CNEPA-NE\ P		1.534	µg/l	1/12/2022 10:49:26
N1030-05 EW2W7S	S	CNEPA-NE\ P		96.7975	µg/l	1/12/2022 10:49:28
N1030-06 EW2Y1	S	CNEPA-NE\ P		0.9104	µg/l	1/12/2022 10:49:29
N1030-07 EW2W8	S	CNEPA-NE\ P		1.8928	µg/l	1/12/2022 10:49:30
N1030-08 EW2W9	S	CNEPA-NE\ P		1.2154	µg/l	1/12/2022 10:49:31
N1030-09 EW2X1	S	CNEPA-NE\ P		2.0088	µg/l	1/12/2022 10:49:32
N1030-10 EW2X3	S	CNEPA-NE\ P		2.8101	µg/l	1/12/2022 10:49:33
PB141966BL PBW966	S	CNEPA-NE\ P		1.6838	µg/l	1/12/2022 10:49:34
N1075-01 EW2W6	S	CNEPA-NE\ P		1.0278	µg/l	1/12/2022 10:49:35
N1075-02 EW310	S	CNEPA-NE\ P		0.7326	µg/l	1/12/2022 10:57:00
N1075-03 EW315	S	CNEPA-NE\ P		1.9035	µg/l	1/12/2022 10:57:01
N1075-04 EW315D	S	CNEPA-NE\ P		1.8418	µg/l	1/12/2022 10:57:02
N1075-05 EW315S	S	CNEPA-NE\ P		96.4588	µg/l	1/12/2022 10:57:04
N1075-06 EW318	S	CNEPA-NE\ P		2.1684	µg/l	1/12/2022 10:57:05
N1075-07 EW319	S	CNEPA-NE\ P		1.2535	µg/l	1/12/2022 10:57:06
N1075-08 EW321	S	CNEPA-NE\ P		2.9415	µg/l	1/12/2022 10:57:07
N1075-09 EW316	S	CNEPA-NE\ P		1.6177	µg/l	1/12/2022 10:57:08
N1075-10 EW317	S	CNEPA-NE\ P		1.1953	µg/l	1/12/2022 10:57:09
CCV002 CCV002	S	CNEPA-NE\ P		245.1075	µg/l	1/12/2022 10:57:10
CCB002 CCB002	S	CNEPA-NE\ P		0.7766	µg/l	1/12/2022 11:00:23

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12 Instrument ID : Konelab

1/12/2022 10:07

Test CNEPA-NEW


Accepted 1/12/2022 10:07

~~Factor~~ Slope 1046 0.000956
Bias Y. Intercept 0.008

12 01/14/22

Coeff. of det. 0.999986

Errors

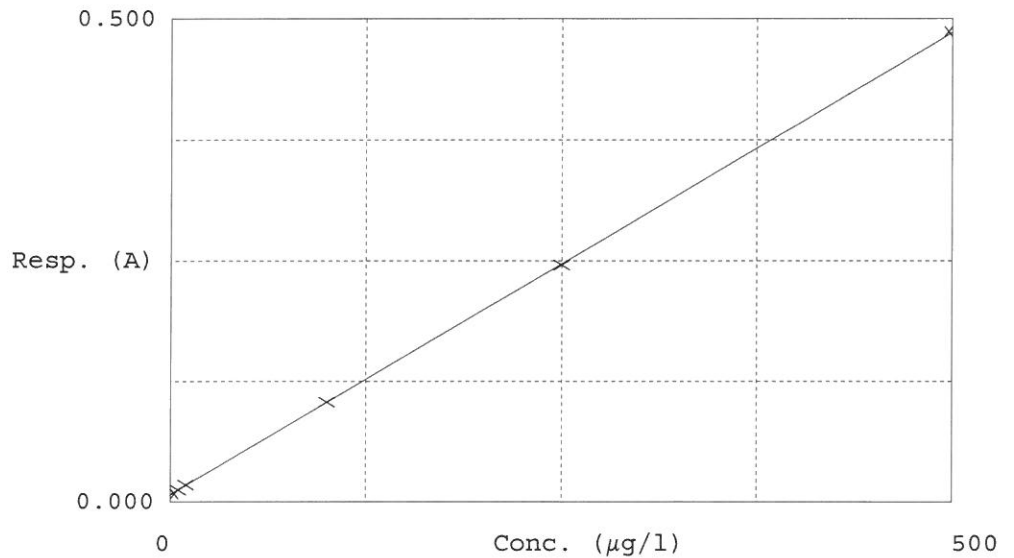

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.008	0.5839	0.0000	-
2	5.0PPBCN	0.012	4.7975	5.0000	-4.0
3	10PPBCN	0.018	10.2529	10.0000	2.5
4	100PPBCN	0.104	100.0789	100.0000	0.1
5	250PPBCN	0.246	248.6111	250.0000	-0.6
6	500PPBCN	0.487	500.6756	500.0000	0.1

12 01/12/22