


LB118250

7471B

INSTRUMENT ID: CV1

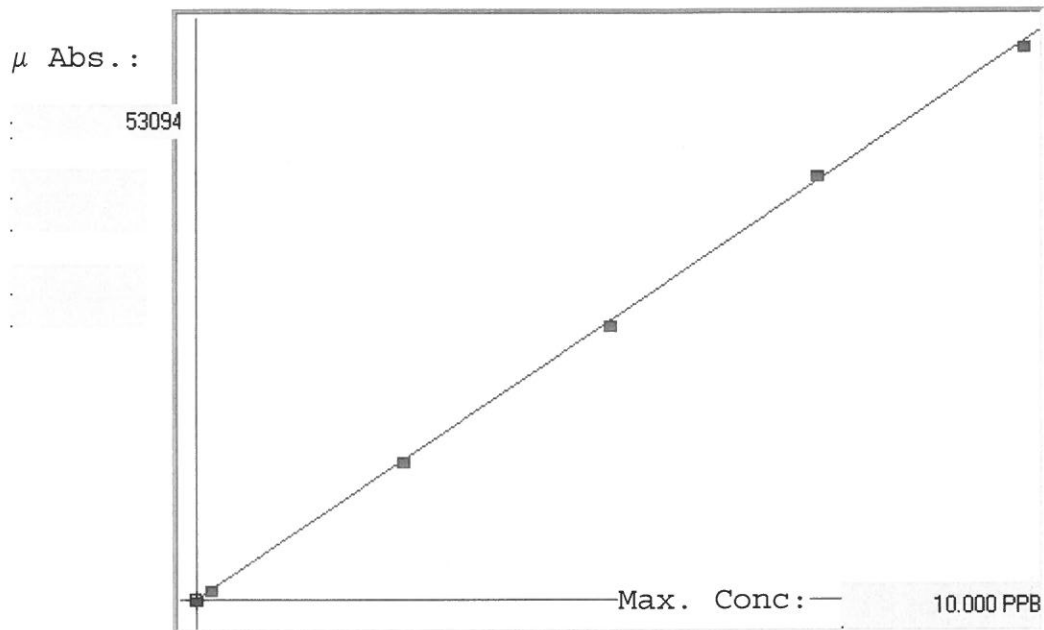

Linear

A= 0.0000e+000

B= 1.8721e-004

C= 7.2802e-003

Rho= 0.9998692

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	0.007	0.007	-4	0.000	-4					-
0.2	0.200	0.208	0.008	1073	0.0 %	1073					4
2.5	2.500	2.491	-0.009	13265	0.0 %	13265					0
5.0	5.000	4.931	-0.069	26300	0.0 %	26300					-1
7.5	7.500	7.617	0.117	40646	0.0 %	40646					2
10.0	10.000	9.947	-0.053	53094	0.0 %	53094					-1

LB118250 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 17 Jan 2022 12:03:51

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	-4	-	0.0000	7471B	PPB	17 Jan 2022 12:05:19	S	Std
0.2 - 1	50.2	1073	-	0.2000	7471B	PPB	17 Jan 2022 12:07:36	S	Std
2.5 - 1	52.5	13265	-	2.5000	7471B	PPB	17 Jan 2022 12:09:53	S	Std
5.0 - 1	55	26300	-	5.0000	7471B	PPB	17 Jan 2022 12:12:10	S	Std
7.5 - 1	57.5	40646	-	7.5000	7471B	PPB	17 Jan 2022 12:19:34	S	Std
10.0 - 1	510	53094	-	10.0000	7471B	PPB	17 Jan 2022 12:24:27	S	Std
ICV48 - 1	ICV48	20146	3.7788	-7471B	PPB	PPB	17 Jan 2022 12:29:39	U	SMPL
ICB48 - 1	ICB48	-87	-0.0090	-7471B	PPB	PPB	17 Jan 2022 12:31:54	U	SMPL
CCV15 - 1	CCV15	24391	4.5735	-7471B	PPB	PPB	17 Jan 2022 12:34:11	U	SMPL
CCB15 - 1	CCB15	-72	-0.0062	-7471B	PPB	PPB	17 Jan 2022 12:36:26	U	SMPL
CRA - 1	CRA	1055	0.2048	-7471B	PPB	PPB	17 Jan 2022 12:38:43	U	SMPL
HighStd - 1	HighStd	50320	9.4277	-7471B	PPB	PPB	17 Jan 2022 12:40:58	U	SMPL
ChkStd - 1	ChkStd	34530	6.4717	-7471B	PPB	PPB	17 Jan 2022 12:43:14	U	SMPL
PB142066BL - 1	PBS	-249	-0.0393	-7471B	PPB	PPB	17 Jan 2022 12:45:31	U	SMPL
PB142066BS - 1	LCSS	19762	3.7069	-7471B	PPB	PPB	17 Jan 2022 12:47:49	U	SMPL
N1086-02 - 1	BBC	3496	0.6618	-7471B	PPB	PPB	17 Jan 2022 12:50:06	U	SMPL
N1152-01 - 1	VACLOT-TOPSOIL-01	2785	0.5287	-7471B	PPB	PPB	17 Jan 2022 12:52:23	U	SMPL
N1158-01 - 1	R-1	5113	0.9645	-7471B	PPB	PPB	17 Jan 2022 12:54:40	U	SMPL
N1164-01 - 1	RBR-251686	10020	1.8831	-7471B	PPB	PPB	17 Jan 2022 12:56:57	U	SMPL
N1164-03 - 1	ETGI-350	20572	3.8586	-7471B	PPB	PPB	17 Jan 2022 12:59:12	U	SMPL
CCV16 - 1	CCV16	24573	4.6076	-7471B	PPB	PPB	17 Jan 2022 13:01:28	U	SMPL
CCB16 - 1	CCB16	-84	-0.0084	-7471B	PPB	PPB	17 Jan 2022 13:03:44	U	SMPL
N1165-01 - 1	NB-07-011422	771	0.1516	-7471B	PPB	PPB	17 Jan 2022 13:06:01	U	SMPL
N1166-01 - 1	SU-01-011422	1110	0.2151	-7471B	PPB	PPB	17 Jan 2022 13:08:16	U	SMPL
N1166-03 - 1	SU-03-011422	1075	0.2085	-7471B	PPB	PPB	17 Jan 2022 13:10:31	U	SMPL
N1166-03DUP - 1	SU-03-011422DUP	996	0.1937	-7471B	PPB	PPB	17 Jan 2022 13:12:47	U	SMPL
N1166-03MS - 1	SU-03-011422MS	20744	3.8908	-7471B	PPB	PPB	17 Jan 2022 13:15:03	U	SMPL
N1166-03MSD - 1	SU-03-011422MSD	19823	3.7184	-7471B	PPB	PPB	17 Jan 2022 13:19:53	U	SMPL
N1166-03LX5 - 1		123	0.0303	-7471B	PPB	PPB	17 Jan 2022 13:22:10	U	SMPL
N1166-03A - 1		22980	4.3094	-7471B	PPB	PPB	17 Jan 2022 13:24:28	U	SMPL
CCV17 - 1	CCV17	26754	5.0159	-7471B	PPB	PPB	17 Jan 2022 13:26:45	U	SMPL
CCB17 - 1	CCB17	-109	-0.0131	-7471B	PPB	PPB	17 Jan 2022 13:29:01	U	SMPL