

LB 118258

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

1/17/2022 15:18

Reviewed by : 12 Instrument ID : Konelab

Test: CNEPA-NEW

Sample Id	^{imp/L} Result	Dil. 1 +	Response	Errors
ICV001 ICV001	93.718	0.0	0.096	
ICB001 ICB001	0.453	0.0	0.007	
CCV001 CCV001	240.839	0.0	0.236	
CCB001 CCB001	0.616	0.0	0.008	
PB142068BL PBS068	0.881	0.0	0.008	
N1135-22 X3884	99.462	0.0	0.102	
N1135-23 X3884D	100.578	0.0	0.103	
N1135-24 X3884S	198.721	0.0	0.196	
PB142069BL PBW069	0.868	0.0	0.008	
N1135-10 X3880	101.583	0.0	0.104	
N1135-11 X3880D	103.643	0.0	0.106	
N1135-12 X3880S	199.908	0.0	0.197	
CCV002 CCV002	246.324	0.0	0.242	
CCB002 CCB002	1.417	0.0	0.008	

12
01/17/22

N	14
Mean	99.215
SD	92.0610
CV%	92.79

Aquakem v. 7.2AQ1

Results from time period:

Mon Jan 17 13:53:18 2022

Mon Jan 17 15:16:39 2022

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time
S0.0	A	CNEPA-NE\ P		-0.1711	µg/l	1/17/2022 13:53:18
S5.0	A	CNEPA-NE\ P		4.9399	µg/l	1/17/2022 13:53:19
S10.0	A	CNEPA-NE\ P		9.8867	µg/l	1/17/2022 13:53:20
S100.0	A	CNEPA-NE\ P		98.821	µg/l	1/17/2022 13:53:21
S250.0	A	CNEPA-NE\ P		252.5695	µg/l	1/17/2022 13:53:22
S500.0	A	CNEPA-NE\ P		498.9539	µg/l	1/17/2022 13:53:23
ICV001 ICV001	S	CNEPA-NE\ P		93.7181	µg/l	1/17/2022 14:23:56
ICB001 ICB001	S	CNEPA-NE\ P		0.453	µg/l	1/17/2022 14:23:58
CCV001 CCV001	S	CNEPA-NE\ P		240.8387	µg/l	1/17/2022 15:09:23
CCB001 CCB001	S	CNEPA-NE\ P		0.6161	µg/l	1/17/2022 15:09:25
PB142068BL PBS068	S	CNEPA-NE\ P		0.8811	µg/l	1/17/2022 15:09:26
N1135-22 X3884	S	CNEPA-NE\ P		99.4617	µg/l	1/17/2022 15:09:29
N1135-23 X3884D	S	CNEPA-NE\ P		100.5781	µg/l	1/17/2022 15:09:30
N1135-24 X3884S	S	CNEPA-NE\ P		198.7206	µg/l	1/17/2022 15:09:32
PB142069BL PBW069	S	CNEPA-NE\ P		0.8679	µg/l	1/17/2022 15:16:31
N1135-10 X3880	S	CNEPA-NE\ P		101.5828	µg/l	1/17/2022 15:16:32
N1135-11 X3880D	S	CNEPA-NE\ P		103.6433	µg/l	1/17/2022 15:16:34
N1135-12 X3880S	S	CNEPA-NE\ P		199.9085	µg/l	1/17/2022 15:16:36
CCV002 CCV002	S	CNEPA-NE\ P		246.3243	µg/l	1/17/2022 15:16:38
CCB002 CCB002	S	CNEPA-NE\ P		1.4174	µg/l	1/17/2022 15:16:39

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

1/17/2022 13:54

Reviewed by : 12 Instrument ID : Konelab

Test CNEPA-NEW


Accepted 1/17/2022 13:53

~~Factor~~ *Slope* ~~1050~~ *0.000953*
~~Bias~~ *Y Intercept* 0.007

12 01/21/22

Coeff. of det. 0.999954

Errors

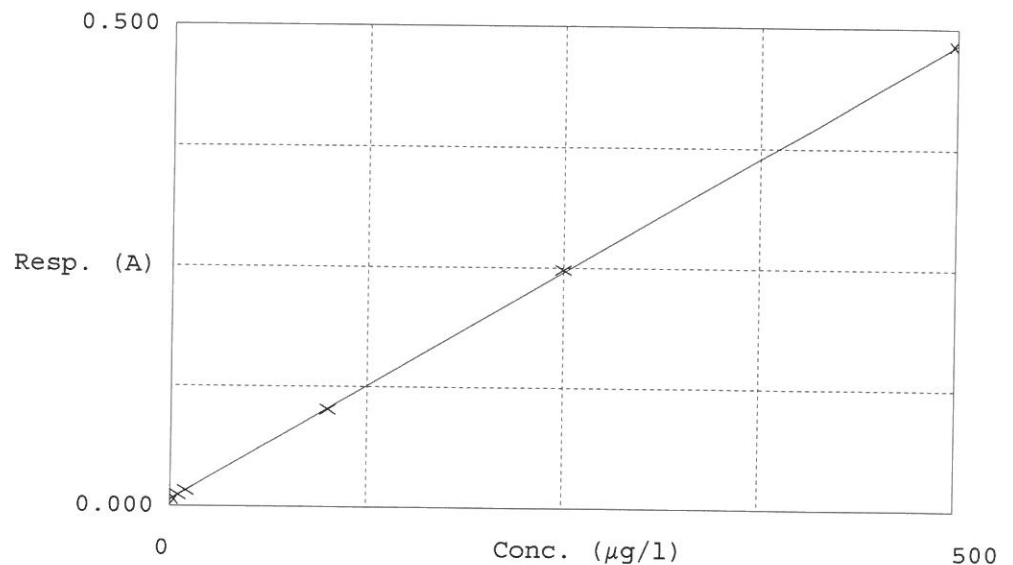

	Calibrator	Response	Calc. con.	Conc.	<i>pe</i> Errors
1	0.0PPBCN	0.007	-0.1711	0.0000	-
2	5.0PPBCN	0.012	4.9399	5.0000	-1.2
3	10PPBCN	0.016	9.8867	10.0000	-1.1
4	100PPBCN	0.101	98.8210	100.0000	-1.2
5	250PPBCN	0.248	252.5695	250.0000	1.0
6	500PPBCN	0.482	498.9539	500.0000	-0.2

01/17/22