

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

1/17/2022 16:23

Reviewed by : 12 Instrument ID : Konelab

Test: Phenolics-

Sample Id	^{mp/L} Result	Dil. 1 +	Response	Errors
ICV1	1.007	0.0	0.116	
ICB1	0.007	0.0	0.004	
CCV1	1.013	0.0	0.117	
CCB1	0.008	0.0	0.004	
PB142067BL	0.005	0.0	0.004	
PB142067BS	1.012	0.0	0.117	
N1147-02	0.017	0.0	0.005	
N1147-02DUP	0.016	0.0	0.005	
N1147-02MS	0.012	0.0	0.005	
N1147-02MSD	1.056	0.0	0.122	
N1147-04	1.030	0.0	0.119	
CCV2	1.005	0.0	0.116	
CCB2	0.008	0.0	0.004	

N 13
Mean 0.477
SD 0.5244
CV% 110.03

Aquakem v. 7.2AQ1

Results from time period:

Mon Jan 17 15:49:51 2022

Mon Jan 17 16:20:58 2022

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.00PPM	A	Phenolics-	P	0.0066	mg/l	1/17/2022 15:49:51	
0.05PPM	A	Phenolics-	P	0.0551	mg/l	1/17/2022 15:49:52	
0.1PPM	A	Phenolics-	P	0.1028	mg/l	1/17/2022 15:49:53	
0.25PPM	A	Phenolics-	P	0.2538	mg/l	1/17/2022 15:49:54	
0.50PPM	A	Phenolics-	P	0.5032	mg/l	1/17/2022 15:49:55	
1.0PPM	A	Phenolics-	P	0.96	mg/l	1/17/2022 15:49:56	
2.0PPM	A	Phenolics-	P	2.0184	mg/l	1/17/2022 15:49:57	
ICV1	S	Phenolics-	P	1.0075	mg/l	1/17/2022 16:15:32	
ICB1	S	Phenolics-	P	0.0069	mg/l	1/17/2022 16:15:34	
CCV1	S	Phenolics-	P	1.0133	mg/l	1/17/2022 16:15:36	
CCB1	S	Phenolics-	P	0.0075	mg/l	1/17/2022 16:15:39	
PB142067BL	S	Phenolics-	P	0.0051	mg/l	1/17/2022 16:15:40	
PB142067BS	S	Phenolics-	P	1.0125	mg/l	1/17/2022 16:15:41	
N1147-02	S	Phenolics-	P	0.0166	mg/l	1/17/2022 16:15:42	
N1147-02DUP	S	Phenolics-	P	0.0163	mg/l	1/17/2022 16:15:43	
N1147-02MS	S	Phenolics-	P	0.0121	mg/l	1/17/2022 16:20:54	
N1147-02MSD	S	Phenolics-	P	1.0559	mg/l	1/17/2022 16:20:55	
N1147-04	S	Phenolics-	P	1.0298	mg/l	1/17/2022 16:20:56	
CCV2	S	Phenolics-	P	1.0052	mg/l	1/17/2022 16:20:57	
CCB2	S	Phenolics-	P	0.0076	mg/l	1/17/2022 16:20:58	

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

1/17/2022 15:51 Reviewed by : 12 Instrument ID : Konelab


Test Phenolics-

Accepted 1/17/2022 15:51

Factor 8.946
Bias 0.004

Coeff. of det. 0.999353

Errors

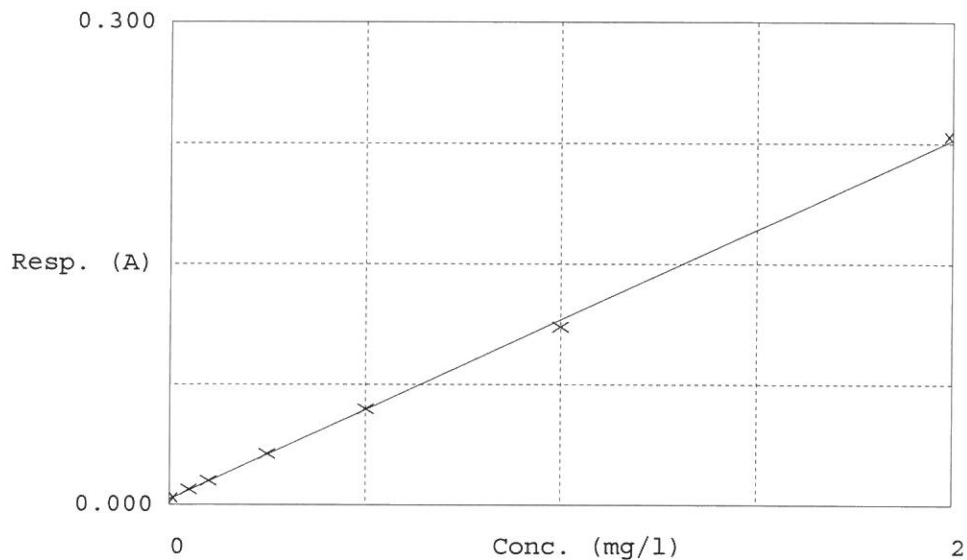

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.00PPM	0.004	0.0066	0.0000	-
2	Phenol-2	0.010	0.0551	0.0500	10.2
3	Phenol-2	0.015	0.1028	0.1000	2.8
4	Phenol-2	0.032	0.2538	0.2500	1.5
5	Phenol-2	0.060	0.5032	0.5000	0.6
6	Phenol-2	0.111	0.9600	1.0000	-4.0
7	Phenol-2	0.229	2.0184	2.0000	0.9

12 01/17/22