

LB 118276

Test results Aquakem 7.2AQ1 Page: 1

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : i2 Instrument ID : Konelab

1/18/2022 15:30

Test: Total CN

Sample Id	^{mp/L} Result	Dil. 1 +	Response	Errors
ICV1	94.387	0.0	0.073	
ICB1	0.420	0.0	0.001	
CCV1	247.313	0.0	0.191	
CCB1	0.430	0.0	0.001	
PB124106BL ^{12/21/06} 12/21/06	0.681	0.0	0.001	
PB142106BS	95.928	0.0	0.074	
N1154-09	^{12/01/18/22} 8.243	0.0	0.007	
N1154-09DUP	7.966	0.0	0.007	
N1154-09MS	38.031	0.0	0.030	
N1154-09MSD	38.296	0.0	0.030	
N1154-10	0.234	0.0	0.001	
CCV2	253.509	0.0	0.196	
CCB2	0.388	0.0	0.001	

N 13
Mean 60.448
SD 90.8686
CV% 150.33

Aquakem v. 7.2AQ1

Results from time period:

Tue Jan 18 15:18:23 2022

Tue Jan 18 15:24:41 2022

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Total CN	P	0.5104	µg/l	1/18/2022 11:09:03	
5.OPPBCN	A	Total CN	P	4.8921	µg/l	1/18/2022 11:09:04	
10PPBCN	A	Total CN	P	9.6738	µg/l	1/18/2022 11:09:05	
50PPBCN	A	Total CN	P	47.8316	µg/l	1/18/2022 11:09:06	
100PPBCN	A	Total CN	P	99.3504	µg/l	1/18/2022 11:09:07	
250PPBCN	A	Total CN	P	254.7748	µg/l	1/18/2022 11:09:08	
500PPBCN	A	Total CN	P	497.9669	µg/l	1/18/2022 11:09:09	
ICV1	S	Total CN	P	94.3868	µg/l	1/18/2022 15:18:23	
ICB1	S	Total CN	P	0.4195	µg/l	1/18/2022 15:18:25	
CCV1	S	Total CN	P	247.3127	µg/l	1/18/2022 15:18:28	
CCB1	S	Total CN	P	0.4297	µg/l	1/18/2022 15:18:30	
PB142106BL	S	Total CN	P	0.6805	µg/l	1/18/2022 15:18:31	
PB142106BS	S	Total CN	P	95.9277	µg/l	1/18/2022 15:18:32	
N1154-09	S	Total CN	P	8.2429	µg/l	1/18/2022 15:18:33	
N1154-09DUP	S	Total CN	P	7.9658	µg/l	1/18/2022 15:24:34	
N1154-09MS	S	Total CN	P	38.0311	µg/l	1/18/2022 15:24:37	
N1154-09MSD	S	Total CN	P	38.2964	µg/l	1/18/2022 15:24:38	
N1154-10	S	Total CN	P	0.2343	µg/l	1/18/2022 15:24:39	
CCV2	S	Total CN	P	253.509	µg/l	1/18/2022 15:24:40	
CCB2	S	Total CN	P	0.3881	µg/l	1/18/2022 15:24:41	

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12 Instrument ID : Konelab

1/18/2022 11:15


Test Total CN

Accepted 1/18/2022 11:11

Factor 1296
Bias 0

Coeff. of det. 0.999842

Errors

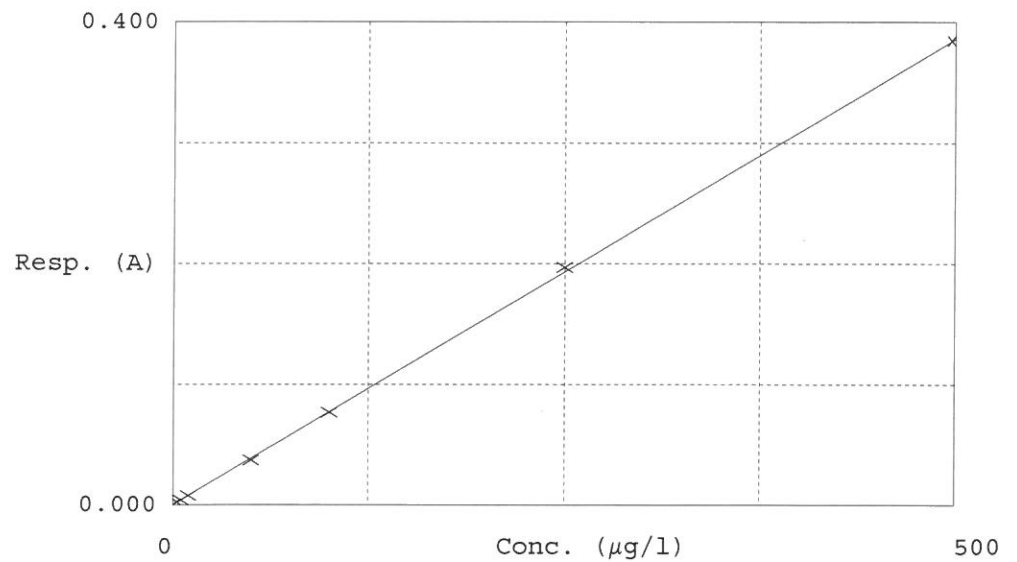

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.001	0.5104	0.0000	-
2	5.0PPBCN	0.004	4.8921	5.0000	-2.2
3	10PPBCN	0.008	9.6738	10.0000	-3.3
4	50PPBCN	0.037	47.8316	50.0000	-4.3
5	100PPBCN	0.077	99.3504	100.0000	-0.6
6	250PPBCN	0.197	254.7748	250.0000	1.9
7	500PPBCN	0.385	497.9669	500.0000	-0.4

12 01/18/22