

LB118303

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12 Instrument ID : Konelab

1/20/2022 12:29

Test: Total CN

Sample Id	^{mp/L} Result	Dil. 1 +	Response	Errors
ICV1	94.313	0.0	0.074	
ICB1	0.491	0.0	0.001	
CCV1	241.448	0.0	0.189	
CCB1	0.336	0.0	0.001	
PB142150BL	0.770	0.0	0.001	
N1186-02	0.443	0.0	0.001	
N1186-02DUP	0.508	0.0	0.001	
N1186-03	0.395	0.0	0.001	
N1186-04	0.275	0.0	0.001	
N1186-05	0.256	0.0	0.001	
N1186-08	0.379	0.0	0.001	
N1188-02	0.516	0.0	0.001	
CCV2	249.381	0.0	0.195	
CCB2	0.616	0.0	0.001	

N	14
Mean	42.152
SD	89.6620
CV%	212.71

Aquakem v. 7.2AQ1

Results from time period:

Thu Jan 20 11:35:40 2022

Thu Jan 20 12:26:32 2022

Sample Id	Sam/Ctr/c	Test short	Test type	Result	Result unit	Result date and time	Stat
0.0PPBCN	A	Total CN	P	0.8959	µg/l	1/20/2022 11:57:08	
5.0PPBCN	A	Total CN	P	5.2131	µg/l	1/20/2022 11:57:09	
10PPBCN	A	Total CN	P	9.7461	µg/l	1/20/2022 11:57:10	
50PPBCN	A	Total CN	P	47.9001	µg/l	1/20/2022 11:57:11	
100PPBCN	A	Total CN	P	98.4664	µg/l	1/20/2022 11:57:12	
250PPBCN	A	Total CN	P	254.5176	µg/l	1/20/2022 11:57:13	
500PPBCN	A	Total CN	P	498.2609	µg/l	1/20/2022 11:57:14	
ICV1	S	Total CN	P	94.3133	µg/l	1/20/2022 12:20:44	
ICB1	S	Total CN	P	0.4905	µg/l	1/20/2022 12:20:45	
CCV1	S	Total CN	P	241.448	µg/l	1/20/2022 12:20:48	
CCB1	S	Total CN	P	0.3358	µg/l	1/20/2022 12:20:50	
PB142150BL	S	Total CN	P	0.7703	µg/l	1/20/2022 12:20:51	
N1186-02	S	Total CN	P	0.4431	µg/l	1/20/2022 12:20:52	
N1186-02DUP	S	Total CN	P	0.5083	µg/l	1/20/2022 12:20:53	
N1186-03	S	Total CN	P	0.3946	µg/l	1/20/2022 12:26:26	
N1186-04	S	Total CN	P	0.2753	µg/l	1/20/2022 12:26:27	
N1186-05	S	Total CN	P	0.2559	µg/l	1/20/2022 12:26:28	
N1186-08	S	Total CN	P	0.3793	µg/l	1/20/2022 12:26:29	
N1188-02	S	Total CN	P	0.5162	µg/l	1/20/2022 12:26:30	
CCV2	S	Total CN	P	249.381	µg/l	1/20/2022 12:26:31	
CCB2	S	Total CN	P	0.6157	µg/l	1/20/2022 12:26:32	

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12 Instrument ID : Konelab

1/20/2022 11:58


Test Total CN

Accepted 1/20/2022 11:58

Factor 1282
Bias 0

Coeff. of det. 0.999849

Errors

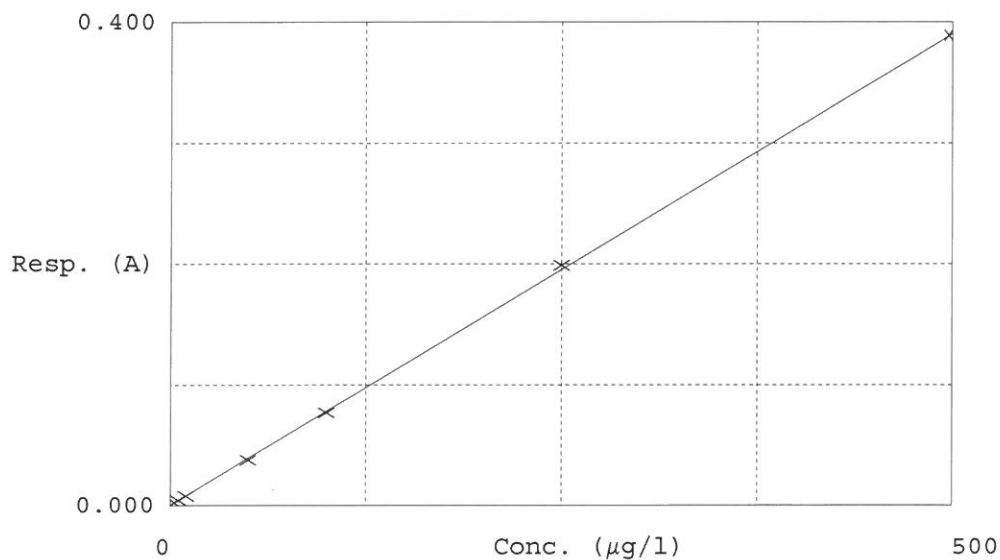

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.001	0.8959	0.0000	-
2	5.0PPBCN	0.004	5.2131	5.0000	4.3
3	10PPBCN	0.008	9.7461	10.0000	-2.5
4	50PPBCN	0.038	47.9001	50.0000	-4.2
5	100PPBCN	0.077	98.4664	100.0000	-1.5
6	250PPBCN	0.199	254.5176	250.0000	1.8
7	500PPBCN	0.389	498.2609	500.0000	-0.3

12 01/20/22